


Purity test of Wood Creosote by Japanese pharmacopoeia

Data No. GA154-0874

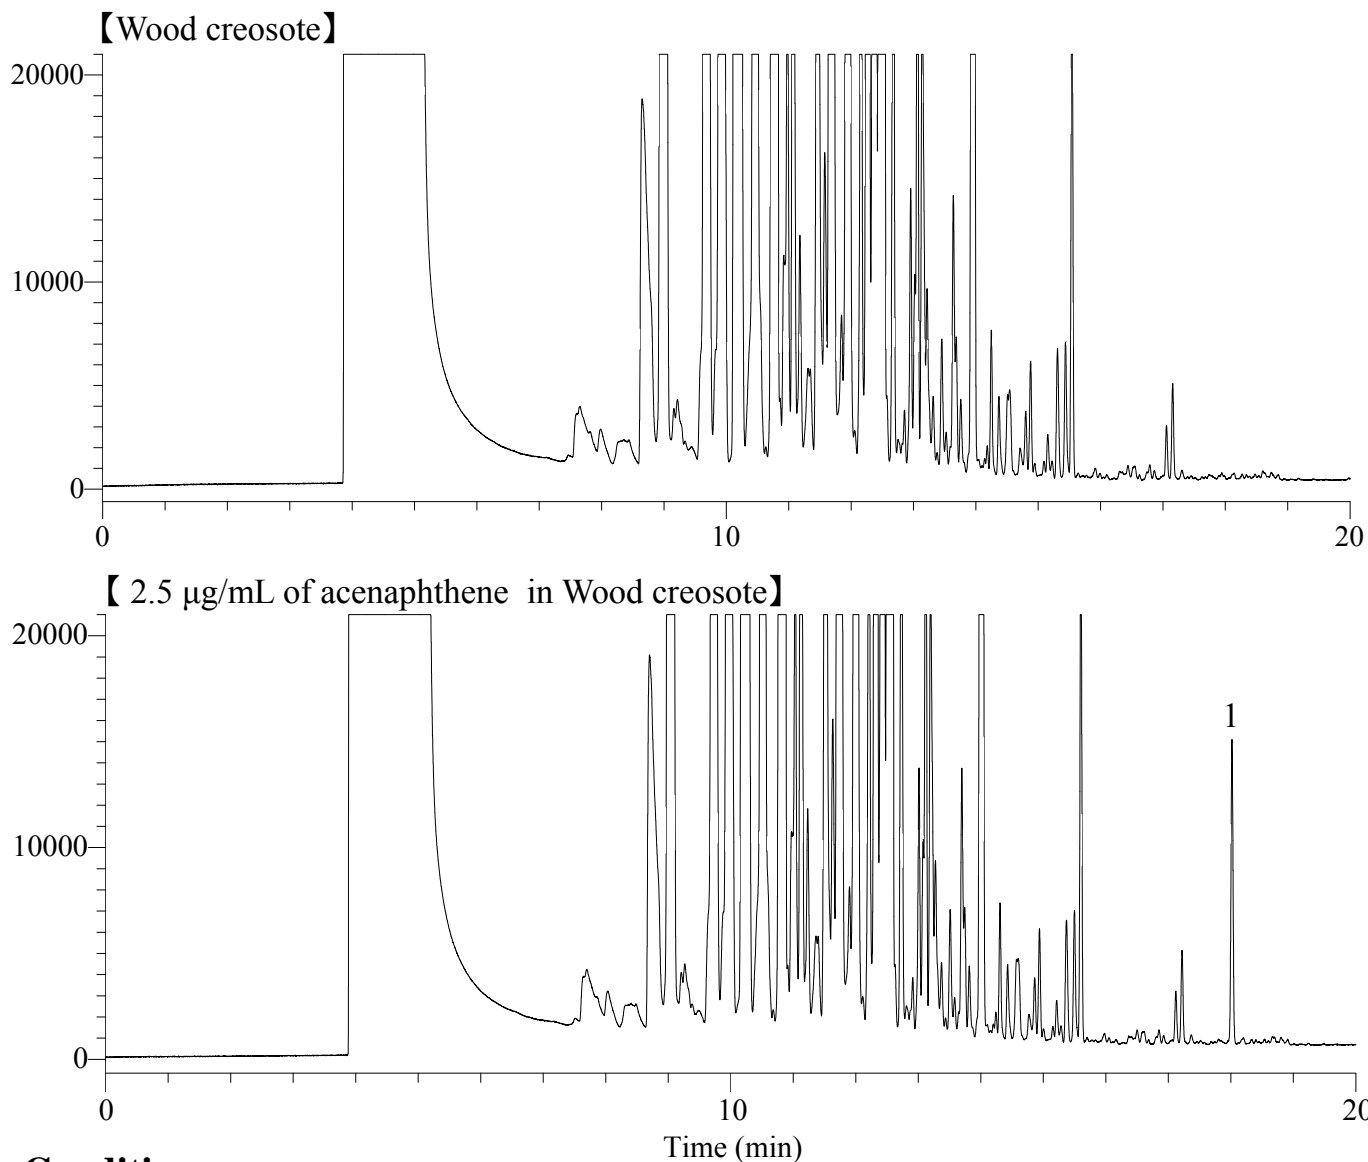

Conditions

System : GC/FID
Column : InertCap 1
0.25 mm I.D. x 60 m df = 0.25 µm
Col. Cat. No. : 1010-11162
Col. Temp. : 45 °C - 11.5 °C/min - 160 °C - 4 °C/min - 180 °C - 8 °C/min - 270 °C(3 min hold)
Carrier Gas : He 220 kPa
Injection : Splitless 1 min Vent flow 20 mL/min
250 °C
Detection : FID Range 10⁰
250 °C
Sample Size : 2.4 mg/mL in Methanol
1.0 µL
Analyte : 1. Acenaphthene 2.5 µg/mL