


Analysis of Nicotinamide

(Under the Condition of USP41-NF36, Oil- and Water-Soluble Vitamins Capsules
NIACINAMIDE_Method 2)

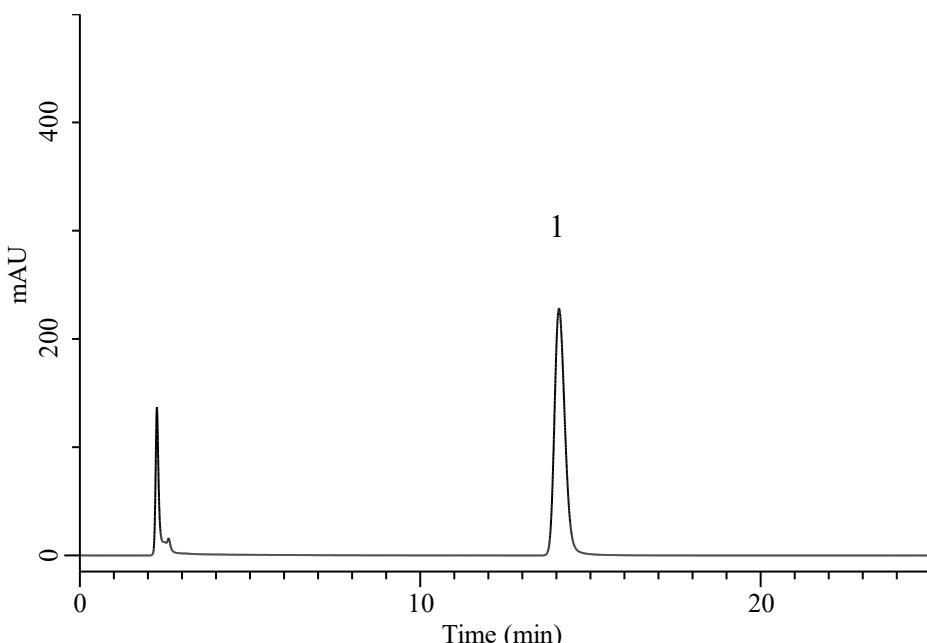

Conditions

System	:	Chromaster PLUS (HITACHI)
Column	:	InertSustain C18 (GL Sciences Inc.) (5 µm, 250 x 4.6 mm I.D.)
Column Cat. No.	:	5020-07346
Eluent	:	Buffer*
Flow Rate	:	1.0 mL/min
Col. Temp.	:	40 °C
Detection	:	UV 254 nm (Chromaster 5420 UV-VIS)
Injection Vol.	:	20 µL
Sample	:	Standard in Solution**/CH ₃ OH=3/1, v/v

Analyte:

1. Nicotinamide 0.2 mg/mL

RSD of the peak area(%) (n=6) : 0.02 (≤ 3.0)

*:13.6 mg/mL of sodium acetate in water. Adjust with acetic acid to a pH of 5.4.

**:Transfer 1 mL of glacial acetic acid and 2.5 g of edetate disodium to a 100-mL volumetric flask. Dissolve in and dilute with water to volume.