


Today, the supply shortage of acetonitrile, which is one of the most widely used organic solvents in HPLC analysis, became extremely hot topic. Raw acetonitrile is obtained as a co-product of acrylonitrile, which is used in automobile component. As a consequence of the global economic recession and the associated reduction of demand for acrylonitrile, there has been a serious decrease in the supply

of acetonitrile.

Methanol, which is also widely used as mobile phase, is easily available at a low price. In this note, how to use methanol instead of acetonitrile is described. What should be paid attention to are elution strength, elution order, and back pressure.

(K.Suzuki)

## < Example 1. >

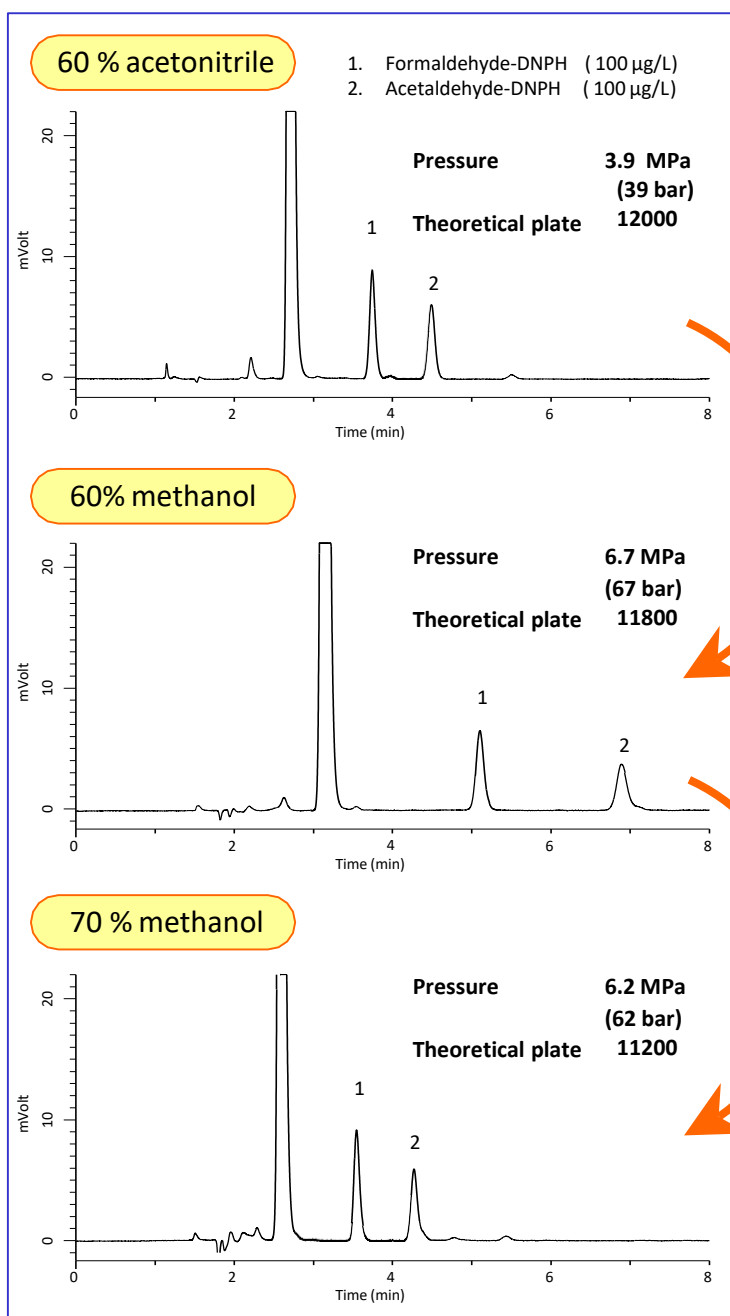

### Conditions

**System** : LC800 HPLC system

**Column** : Inertsil ODS-SP  
(5 µm, 150 × 3.0 mm I.D.)


**Eluent** : CH<sub>3</sub>CN / H<sub>2</sub>O or CH<sub>3</sub>OH / H<sub>2</sub>O

**Flow rate** : 0.4 mL/min

**Col. Temp.** : 60 °C

**Detection** : UV 360 nm

**Inj. Vol.** : 10 µL

 : Mobile phase composition


Elution strength tends to decrease.  
Depending on the samples, the elution order may change.

The back pressure becomes high. (See also next page.)


Methanol concentration should be increased to adjust retention times.

### An indicator for elution strength

With a line perpendicular to the scales below, mobile phase composition which provides similar retention times can be obtained.




Switching from acetonitrile to methanol may cause changes in the elution order as the chromatograms shown below.

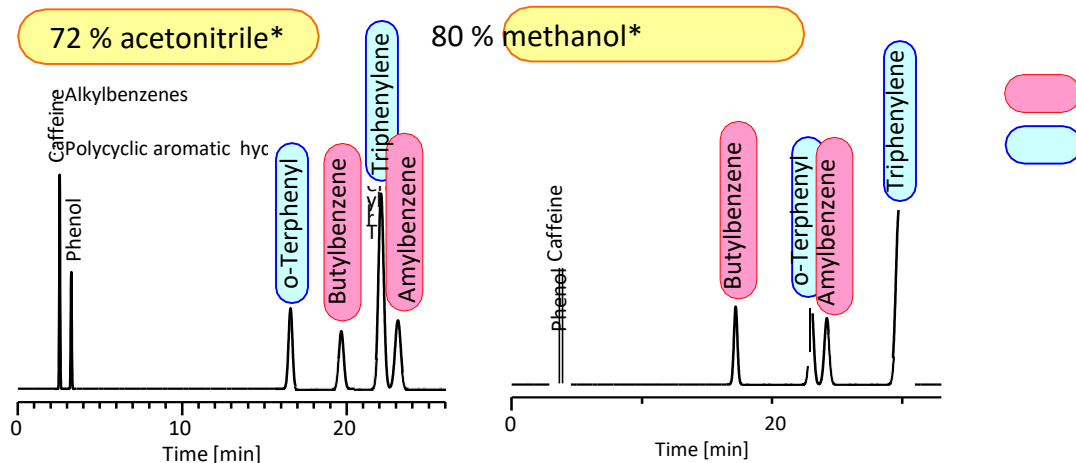

\* The compositions were adjusted to obtain similar retention times.

## Back pressure comparison among commercially available ODS columns

Even among ODS columns with the same specifications (inner diameter, length, and particle size), the column back pressure varies with the packed particles. In case the pressure becomes too high, HPLC system and the column itself may be damaged.

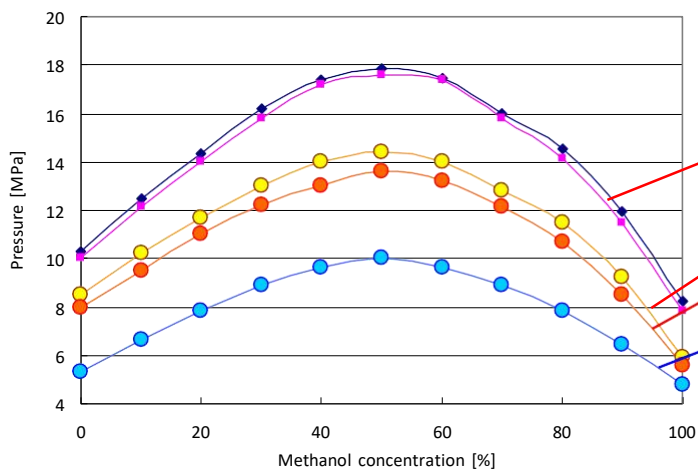

Other ODS columns

Inertsil ODS-4

Inertsil ODS-SP

Inertsil ODS-3

Inertsil series are advantageous in switching to methanol because the columns provide the lowest back pressure in the world!

Column size: 250 × 4.6 mm I.D., 5 μm  
Flow rate: 1.0 mL/min Column Temp.: 40 °C

GL Sciences disclaims any and all responsibility for any injury or damage which may be caused by this data directly or indirectly. We reserve the right to amend this information or data at any time and without any prior announcement.

### GL Sciences, Inc. Japan

22-1 Nishishinjuku 6-Chome  
Shinjuku-ku, Tokyo,  
163-1130, Japan  
Phone: +81-3-5323-6620  
Fax: +81-3-5323-6621  
Email: [world@glsc.co.jp](mailto:world@glsc.co.jp)  
Web: [www.glsciences.com](http://www.glsciences.com)

### GL Sciences B.V.

De Sleutel 9  
5652 AS Eindhoven  
The Netherlands  
Phone: +31 (0)40 254 95 31  
Email: [info@glsciences.eu](mailto:info@glsciences.eu)  
Web: [www.glsciences.eu](http://www.glsciences.eu)

### GL Sciences (ShangHai) Ltd.

Tower B, Room 2003,  
Far East International Plaza,  
NO,317 Xianxia Road,  
Changning District.  
Shanghai, China P.C. 200032  
Phone: +86 (0)21-6278-2272  
Email: [contact@glsciences.com.cn](mailto:contact@glsciences.com.cn)  
Web: [www.glsciences.com.cn](http://www.glsciences.com.cn)

### GL Sciences, Inc. USA

4733 Torrance Blvd. Suite 255  
Torrance, CA 90503  
Phone: 310-265-4424  
Fax: 310-265-4425  
Email: [info@glsciencesinc.com](mailto:info@glsciencesinc.com)  
Web: [www.glsciencesinc.com](http://www.glsciencesinc.com)

### International Distributors

Visit our Website at:  
<https://www.glsciences.com/company/distributor.html>