


Analysis of Spiramycin, Neospiramycin

Data No. LA561-0696

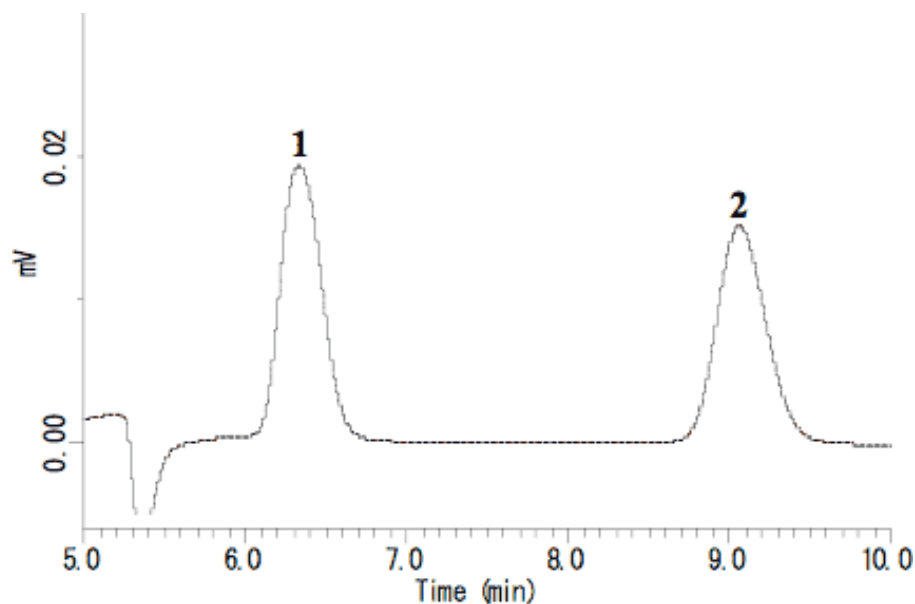

System	: GL-7400 system	Solutes	: 1. Spiramycin (100 μ g/mL)
Column	: Inertsil ODS-3 (5 μ m, 150 \times 4.6 mm I.D.)		2. Neospiramycin (100 μ g/mL)
Column Cat. No.	:		
Eluent	: A) CH ₃ CN B) 65 mM NaH ₂ PO ₄ (pH 2.5; H ₃ PO ₄) A/B = 25/75 ,v/v		
Flow rate	: 400 μ L/min		
Col. Temp.	: 40 $^{\circ}$ C		
Detection	: UV 235 nm (GL-7450 UV Detector)		
Injection Vol.	: 20 μ L		
Sample	:		