


# InertSearch™ for LC

Inertsil® Applications

## Analysis of Urea

Data No. LB108-0848

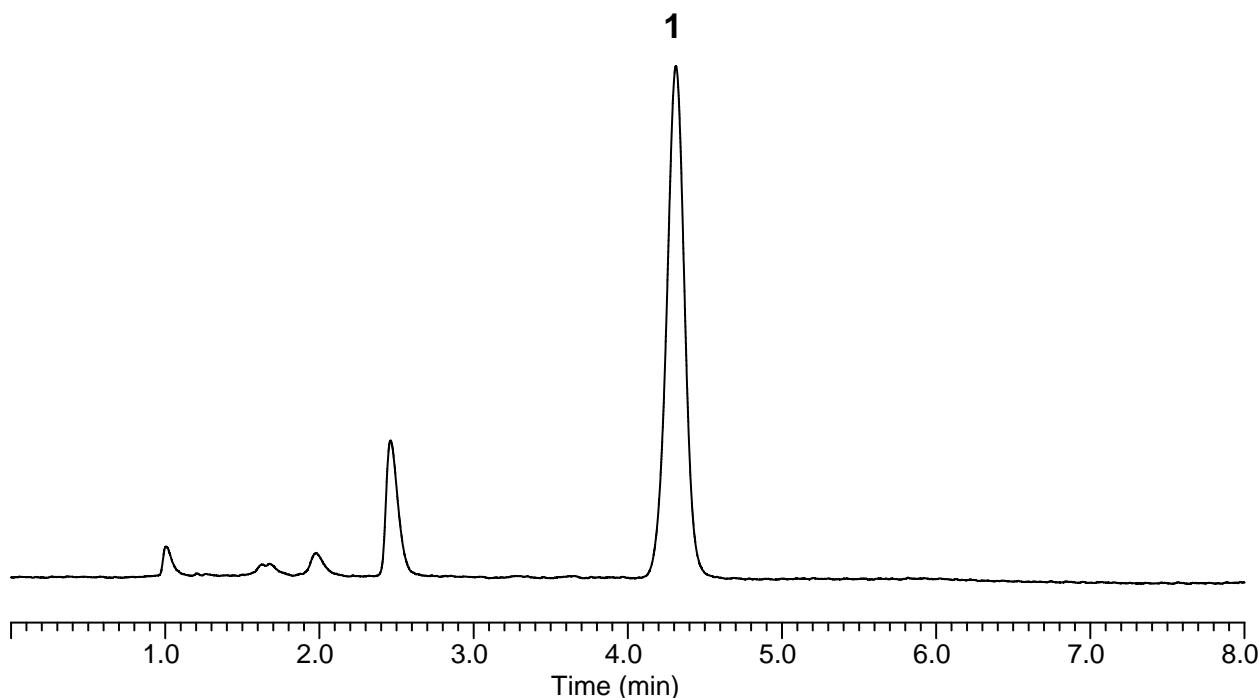

### Conditions

System : LC800 HPLC System  
Column : Inertsil Amide (5 µm, 150 x 3.0 mm I.D.)  
Column Cat. No. : 5020-07815  
Eluent : A) CH<sub>3</sub>CN  
          B) H<sub>2</sub>O  
          A/B = 85/15 , v/v  
Flow Rate : 0.4 mL/min.  
Col. Temp. : 40 °C  
Detection : UV 200 nm  
Injection Vol. : 5.0 µL

### Analyte

1. Urea      200 mg/L