


# InertSearch™ for LC

Inertsil® Applications

## Analysis of Lactosucrose

Data No. LB005-0848

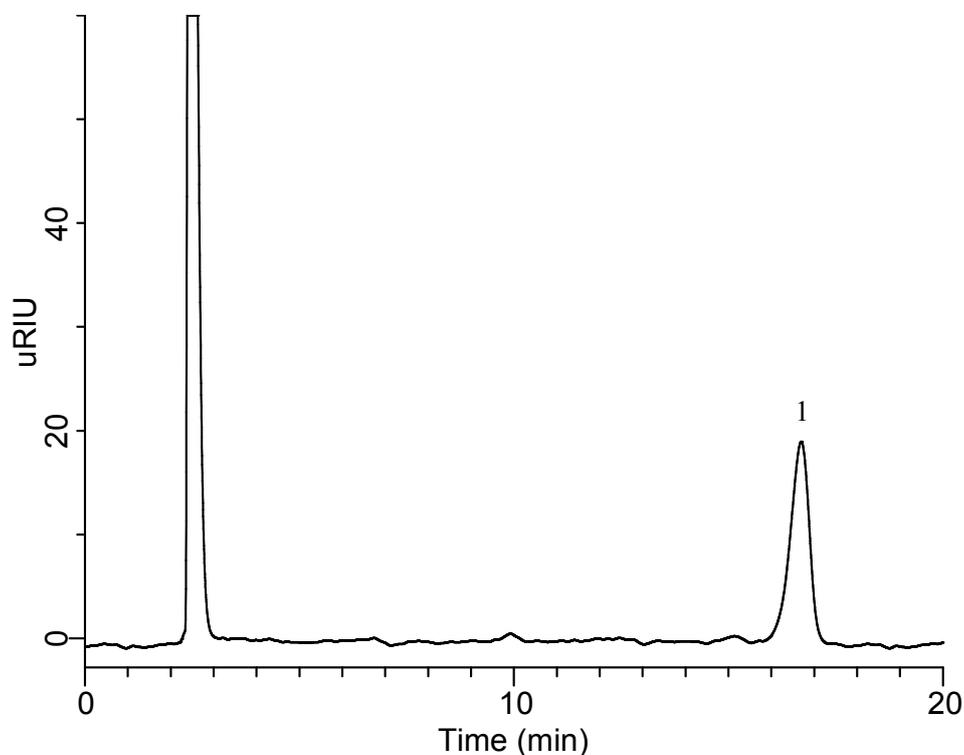


### Conditions

**System** : GL-7400 HPLC system  
**Column** : Inertsil Amide (5 μm, 250 x 4.6 mm I.D.)  
**Column Cat. No.** : 5020-07836  
**Eluent** : A) CH<sub>3</sub>CN  
          : B) H<sub>2</sub>O  
          : A/B = 71/29, v/v  
**Flow rate** : 1.2 mL/min  
**Col. Temp.** : 35 °C  
**Detection** : RI (GL-7454 RI Detector)  
**Injection Vol.** : 20 μL  
**Sample** : Standard

### Analyte:

1. Lactosucrose 5 mg/mL

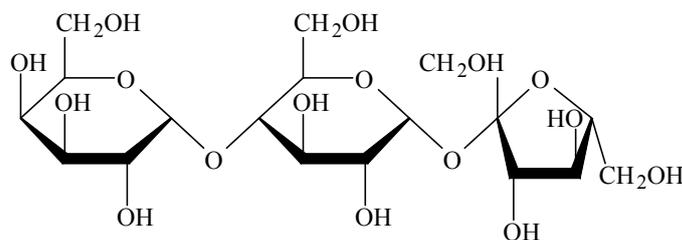

Structures are created using Chemistry 4-D Draw which is provided by ChemInnovation Software, Inc.