


Organic Solvents

Data No. GA 284-0644

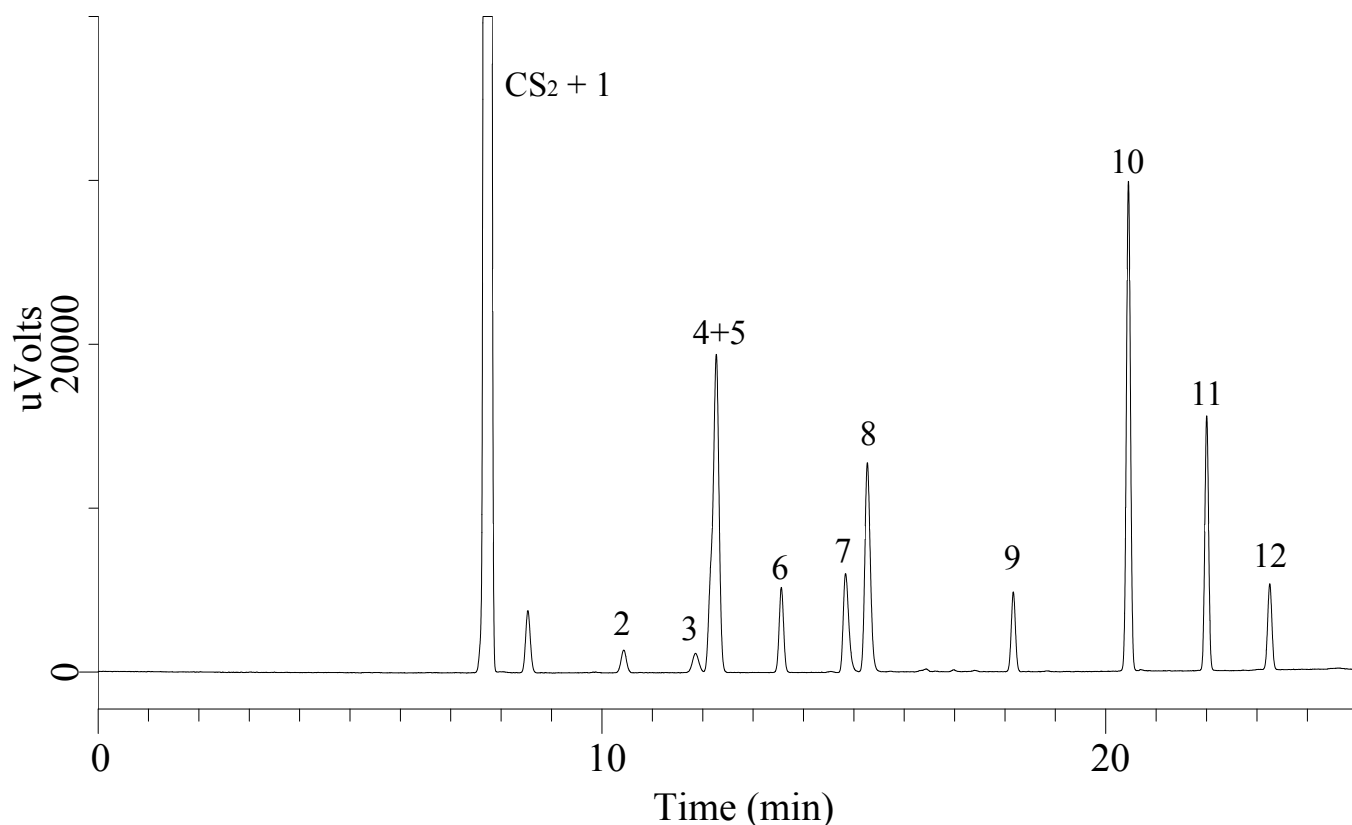

Conditions

System	: GC-FID	Analyte	: 1. Dichloromethane
Column	: InertCap AQUATIC 0.53 mm I.D. x 75 m df = 2.0 µm		: 2. Chloroform
Col. Cat. No.	: 1010-29477		: 3. Carbon tetrachloride
Col. Temp.	: 40 °C (5 min hold) - 5 °C/min - 180 °C		: 4. Benzene
Carrier Gas	: He 5 mL/min		: 5. 1,2-Dichloroethane
Injection	: Split flow 50 mL/min 220 °C		: 6. Trichloroethylene
Detection	: FID Auto Range 220 °C		: 7. 1,4-Dioxane
Sample Size	: 100 µg/mL in Carbon disulfide 1.0 µL		: 8. 4-Methyl-2-pentanone(MIBK)
			: 9. Tetrachloroethylene
			: 10. Ethylbenzene
			: 11. Styrene
			: 12. 1,1,2,2-Tetrachloroethane