


17. Standard Sugars

Data No. LA072-0000

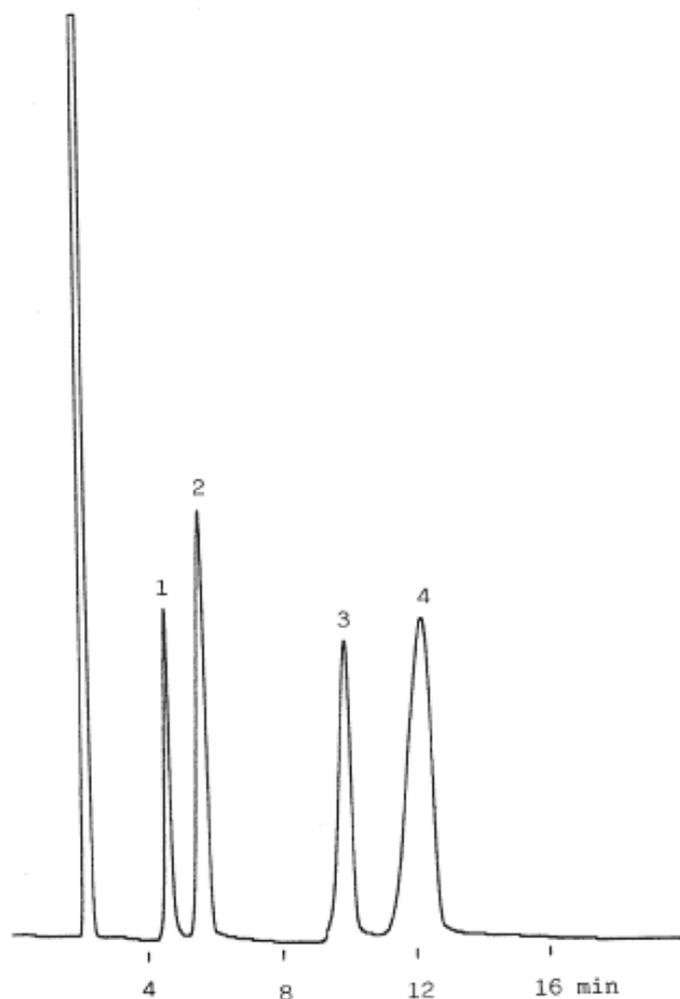

Column : Bioptic AV-2
150 × 4.6 mm I.D.

Column Cat. No. :

Eluent : CH₃CN/H₂O = 90/10

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : RI

Injection Vol. :

Sample : Sugars

Solutes : 1. Fructose
2. Glucose
3. Sucrose
4. Maltose