


InertSearch for LC

Inertsil Applications

Analysis of Glyphosate and Glufosinate

Data No. LB724-0806

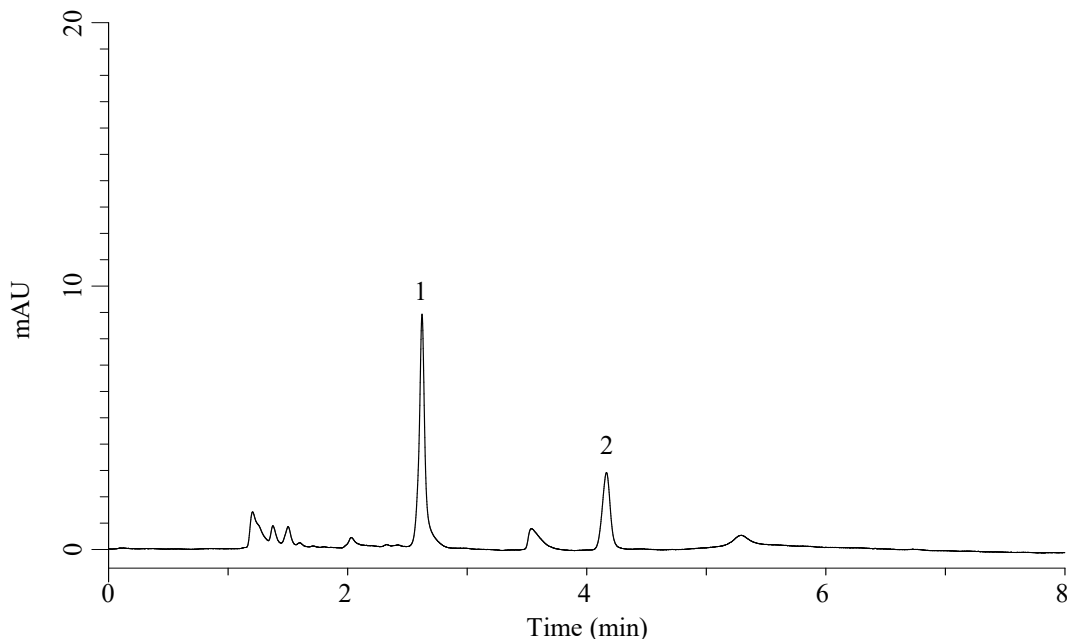

Conditions

System : Chromaster HPLC system (HITACHI)
Column : InertSustain AX-C18 (GL Sciences Inc.)
(3 μ m, 150 x 2.1 mm I.D.)
Column Cat. No. : 5020-91039
Eluent : 0.1% H₃PO₄ in H₂O
Flow Rate : 0.2 mL/min
Col. Temp. : 40 °C
Detection : UV 210 nm
Injection Vol. : 1 μ L
Sample : Standard

Analyte:

1. Glufosinate
2. Glyphosate
(1,000 mg/L each)