


# InertSearch for LC

Inertsil Applications

## Analysis of Per - and Polyfluoroalkyl Substances (PFAS)

Data No. LB707-0888

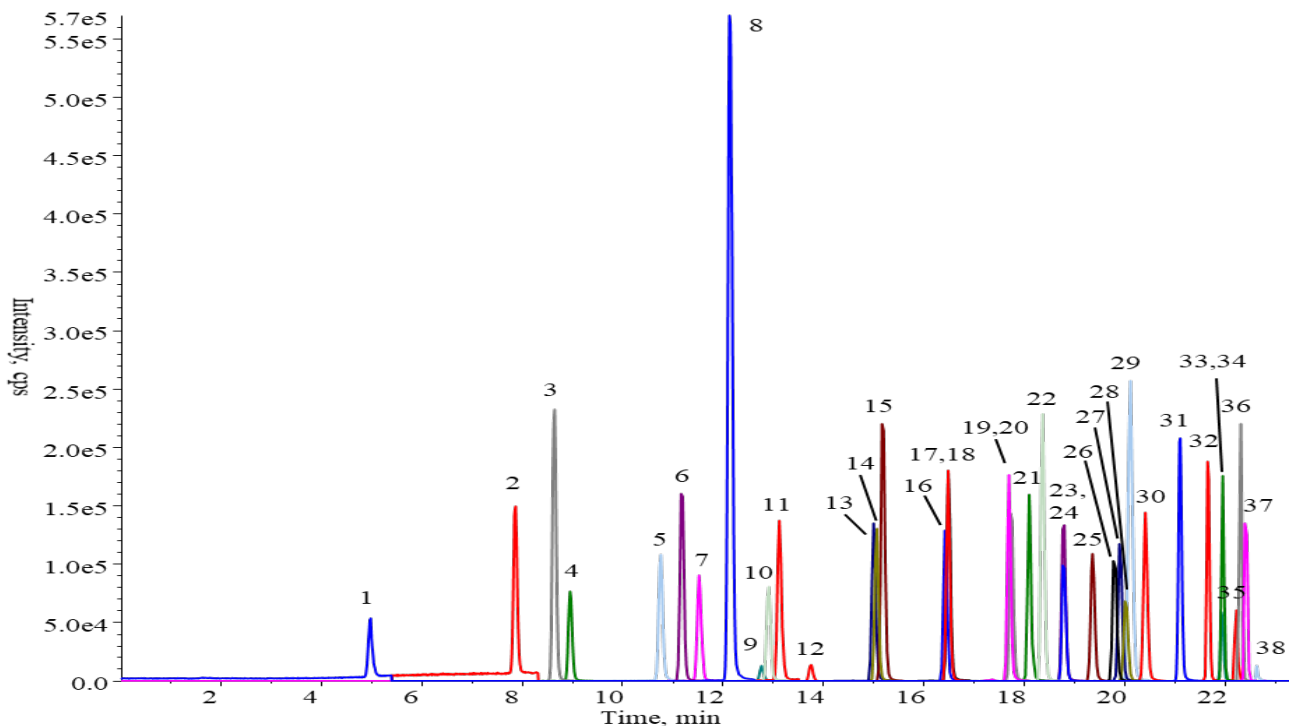

### Conditions

**System** : Exion HPLC System (SCIEX)  
QTRAP 6500+ LC-MS/MS System (SCIEX)

**Column** : InertSustain AQ-C18 (1.9  $\mu\text{m}$ , 100 x 2.1 mm I.D.) (GL Sciences Inc.)

**Column Cat. No.** : 5020-89939

**Delay Column** : Delay Column for PFAS (30 x 3.0 mm I.D.) (GL Sciences Inc.)

**Delay Column Cat. No.** : 5020-90005

**Eluent** : A)  $\text{CH}_3\text{OH}$   
B) 20 mmol/L  $\text{CH}_3\text{COONH}_4$  in  $\text{H}_2\text{O}$

Time (min)	A%	B%
0	5	95
0.5	5	95
3.0	40	60
16.0	80	20
18.0	80	20
20.0	95	5
22.0	95	5
25.0	5	95
35.0	5	95

**Flow Rate** : 0.25 mL/min

**Col. Temp.** : 40  $^\circ\text{C}$

**Detection** : LC/MS/MS (ESI, Negative, SRM)

CUR	CAD	IS	TEM	GS1	GS2
40	12	-4500	300	50	30

**Injection Vol.** : 2  $\mu\text{L}$

**Sample** : Standard in Methanol (1 ng/mL each)

# InertSearch for LC

## Inertsil Applications

No.	Compound	R.T.	Transition 1			Transition 2		
			Q1	Q3	CE	Q1	Q3	CE
1	PFPrA	5.0	163	119	-16			
2	PFBA	7.9	213	169	-14			
3	PFPrS	8.6	249	80	-52	249	99	-34
4	PFMBA	9.0	229	85	-16			
5	PFPeA	10.8	263	219	-11			
6	PFBS	11.2	299	80	-59	299	99	-44
7	PFMPA	11.5	279	85	-14			
8	PFEESA	12.1	315	135	-30	315	83	-24
9	NFDHA	12.8	295	201	-12	295	85	-30
10	4:2 FTSA	12.9	327	307	-28	327	81	-54
11	PFHxA	13.1	313	269	-15	313	119	-30
12	HFPO-DA(GenX)	13.8	329	169	-16	329	285	-8
13	PFHpA	15.0	363	319	-14	363	169	-26
14	PFHxS	15.1	399	80	-80	399	99	-80
15	ADONA(DONA)	15.2	377	251	-14	377	85	-56
16	6:2 FTSA	16.4	427	407	-32	427	81	-72
17	PFOA	16.5	413	369	-14	413	169	-26
18	PFHpS	16.5	449	80	-104	449	99	-70
19	PFOS	17.7	499	80	-97	499	99	-77
20	PFNA	17.8	463	419	-16	463	219	-26
21	8:2 FTUCA	18.1	457	393	-18	457	343	-52
22	9Cl-PF3ONS	18.4	531	351	-40	531	83	-56
23	8:2 FTSA	18.8	527	507	-40	527	81	-82
24	PFDA	18.8	513	469	-19	513	219	-27
25	N-MeFOSAA	19.4	570	419	-28	570	483	-22
26	PFDS	19.8	599	80	-94	599	99	-91
27	PFUnDA(PFUnA)	19.9	563	519	-19	563	269	-28
28	N-EtFOSAA	20.0	584	419	-28	584	526	-22
29	FOSA(PFOSA)	20.1	498	78	-85	498	169	-40
30	10:2 FTUCA	20.4	557	493	-20	557	243	-52
31	PFDoDA(PFDoA)	21.1	613	569	-17	613	269	-29
32	PFTTrDA(PFTTrA)	21.7	663	619	-19	663	269	-32
33	N-MeFOSA	21.9	512	169	-37	512	219	-34
34	PFTeDA(PFTeA)	22.0	713	669	-19	713	319	-36
35	N-EtFOSA	22.2	526	169	-37	526	219	-34
36	PFHxDA	22.3	813	769	-20	813	319	-34
37	8:2 diPAP	22.4	989	97	-88	989	543	-35
38	PFOcDA(PFOcDA)	22.6	913	869	-20	913	369	-40