


## Analysis of VMA, 5-HIAA and HVA

Data No. LA237-0000

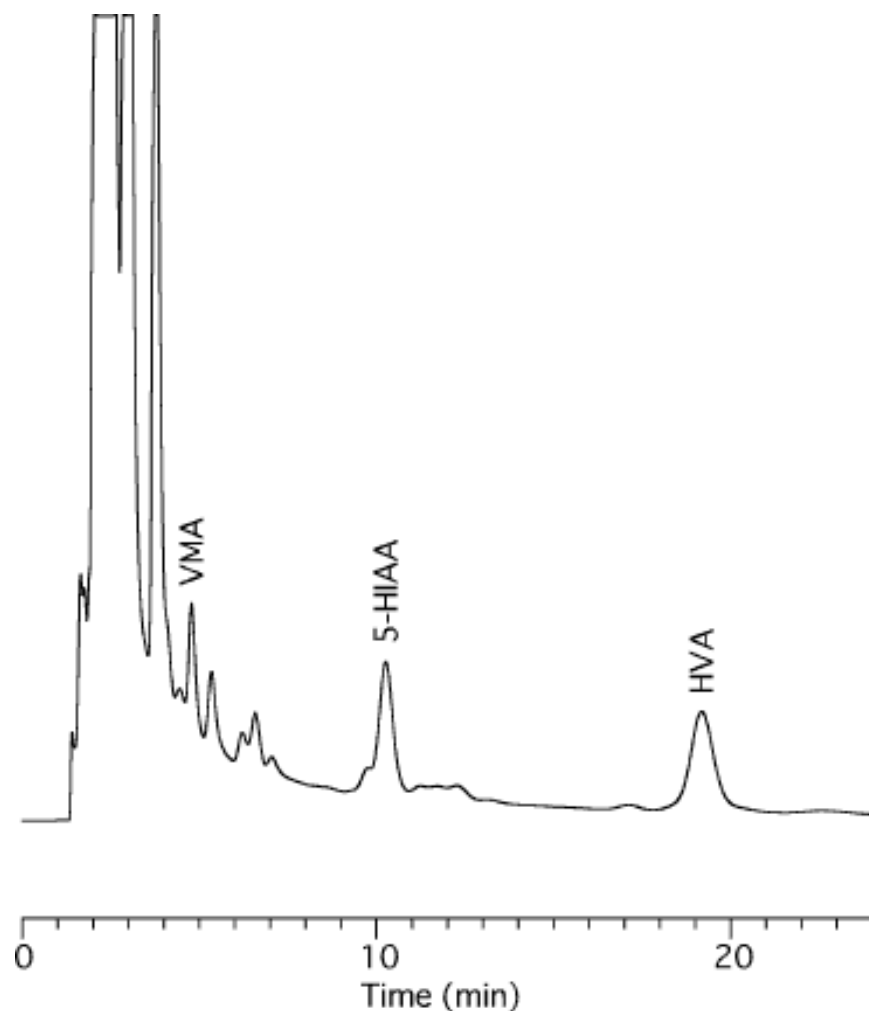

Column :Inertsil CN-3  
5 $\mu$ m  
150  $\times$  4.6mm I.D.

Solutes : 1. VMA  
2. 5-HIAA  
3. HVA

Column Cat. No. :

Eluent :Acetonitrile/50mM phosphate buffer (pH3.0) = 1/99

Flow rate :1mL/min

Col. Temp. :30°C

Detection :ECD 700mV vs. Ag/AgCl

Injection Vol. :10 $\mu$ L

Sample :liquid-liquid extract of urine