


InertSearch™ for GC

InertCap® Applications

Application of the PCB out of the insulating oil after cleaning up Data No. GA013-0000

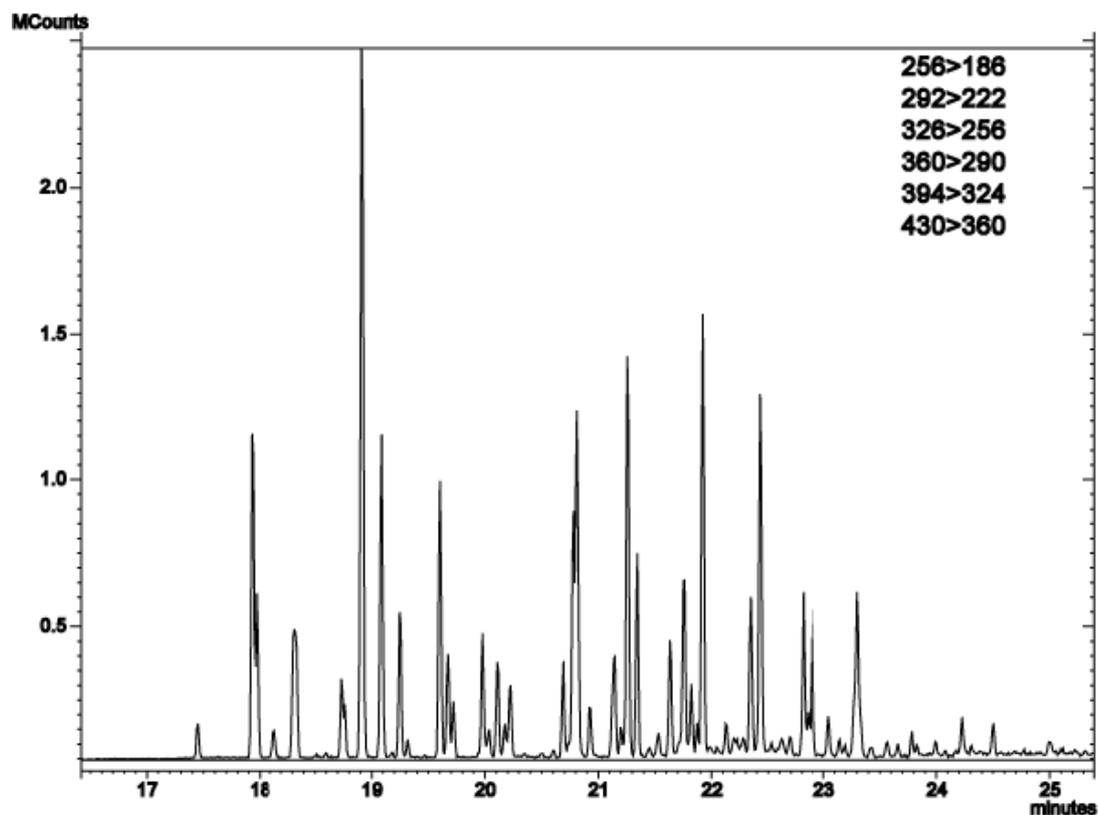

System : GC/MSMS PAC795 OPTIC3
Column : InertCap 5MS/Sil
0.25mmI.D.×30m df=0.25µm
Column Temp. : 50°C (3min)→15°C/min→280°C
Carrier Gas : He
Injection : DMI 2µL
60°C→10°C/sec→280°C
Detection : MS/MS
Collision Gas : Ar
Sample : Insulating oil