


## Analysis of Endocrine disruptors

Data No. LA333-0000

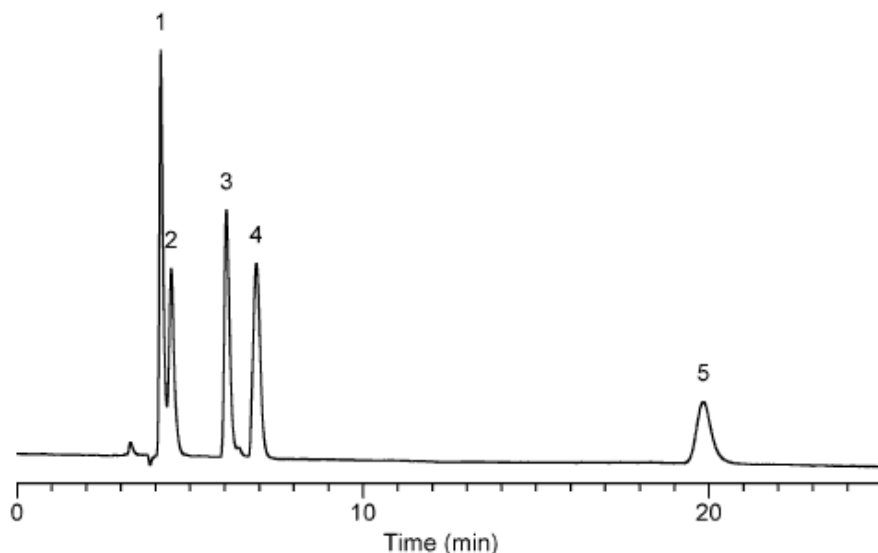

No.	Peak Name	R.Time	Area
1	Diethyl phthalate	4.153	30371
2	4-Nonylphenol	4.453	20231
3	2,4-Dichlorophenol	6.053	26894
4	Phenol	6.917	28500
5	Bisphenol-A	19.840	16911

Column :Inertsil CN-3  
5µm  
250×4.6mmI.D.

Column Cat. No. :

Eluent :hexane / ethanol = 90 / 10

Flow rate :1.0mL/min

Col. Temp. :40°C

Detection :UV 280 nm

Injection Vol. :1µL

Sample :Diethyl phthalate (0.13 mg/mL)  
4-Nonylphenol (0.13 mg/mL)  
2,4-Dichlorophenol (0.065 mg/mL)  
Phenol (0.065 mg/mL)  
Bisphenol-A (0.03 mg/mL)

Solutes : 1. Diethyl phthalate 4.153 30371  
2. 4-Nonylphenol 4.453 20231  
3. 2,4-Dichlorophenol 6.053 26894  
4. Phenol 6.917 28500  
5. Bisphenol-A 19.840 16911