


Analysis of Vitamin D3 in Food

Data No. LA503-0696

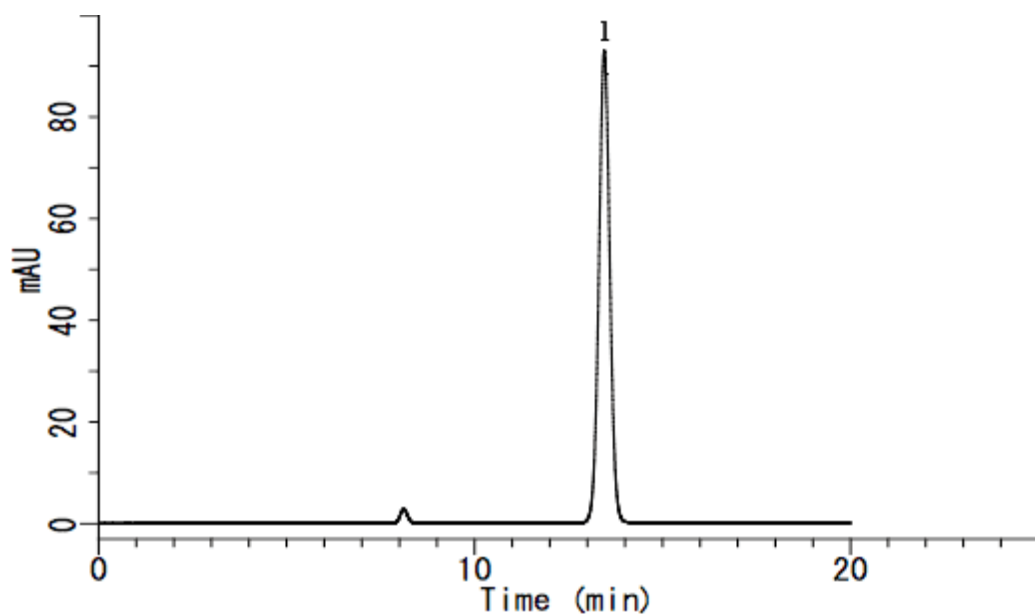

System : GL-7400 system
Column : Inertsil NH2 (5 μ m, 250 \times 10 mm I.D.)
Column Cat. No. :
Eluent : 2-Propanol / n-Hexane = 1 /99 ,v/v
Flow rate : 7 mL/min.
Col. Temp. : 40 $^{\circ}$ C
Detection : UV 265 nm (GL-7450 UV Detector)
Injection Vol. : 500 μ L
Sample :

Solutes : 1. D3 (Cholecalciferol) (10mg/L)