


# InertSearch™ for LC

Inertsil® Applications

## Analysis of Epalrestat

(Under the Condition of the Japanese Pharmacopoeia)

Data No. LB113-0919

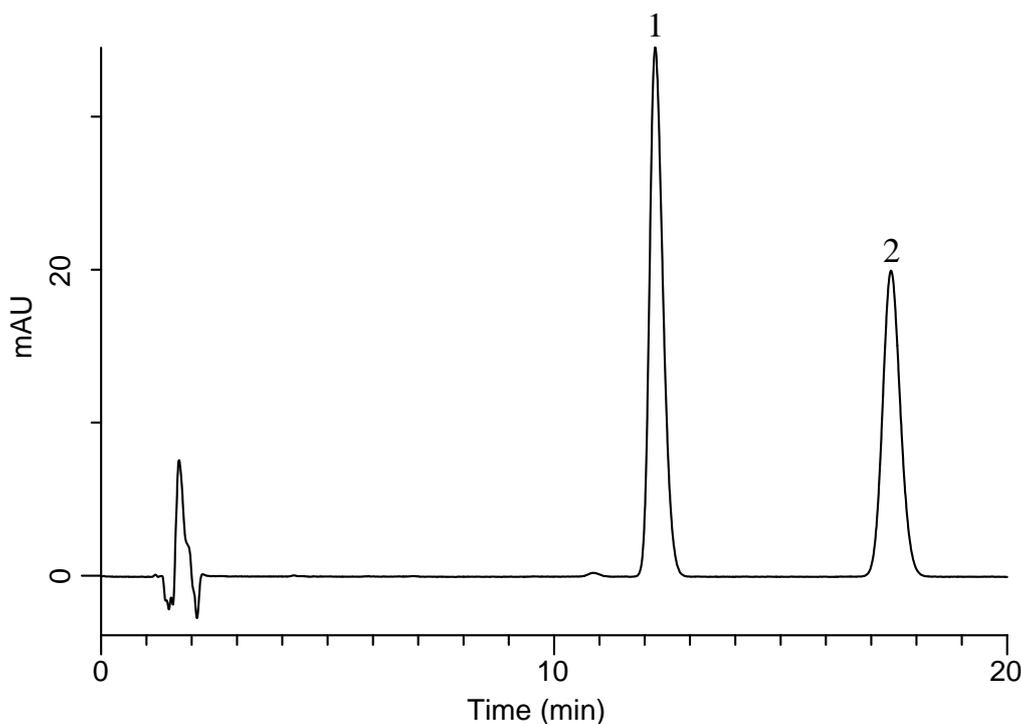

### Conditions

**System** : GL-7400 HPLC system  
**Column** : InertSustain C18  
(5  $\mu$  m, 150 x 4.6 mm I.D.)  
**Column Cat. No.** : 5020-07345  
**Eluent** : A) CH<sub>3</sub>CN  
B) 0.05 mol/L KH<sub>2</sub>PO<sub>4</sub> in H<sub>2</sub>O  
(pH 6.5, 0.05 mol/L Na<sub>2</sub>HPO<sub>4</sub> in H<sub>2</sub>O )  
A/B = 1/2, v/v  
**Flow Rate** : 1.0 mL/min  
**Col. Temp.** : 25 °C  
**Detection** : UV 280 nm (GL-7452 PDA Detector)  
**Injection Vol.** : 3  $\mu$  L  
**Sample** : Standard

### Analyte:

1. Epalrestat 200 mg/L  
2. *p*-Hydroxybenzoic acid *n*-propyl ester 200 mg/L

Resolution (1, 2) : 8.31 ( $\geq$  2.0)  
RSD of the peak  
area ratio of  
1 to 2 (%) (n=6) : 0.20 ( $\leq$  1.0)