


# InertSearch™ for LC

Inertsil® Applications

## Insulin standards E10

Data No. LA137-0000

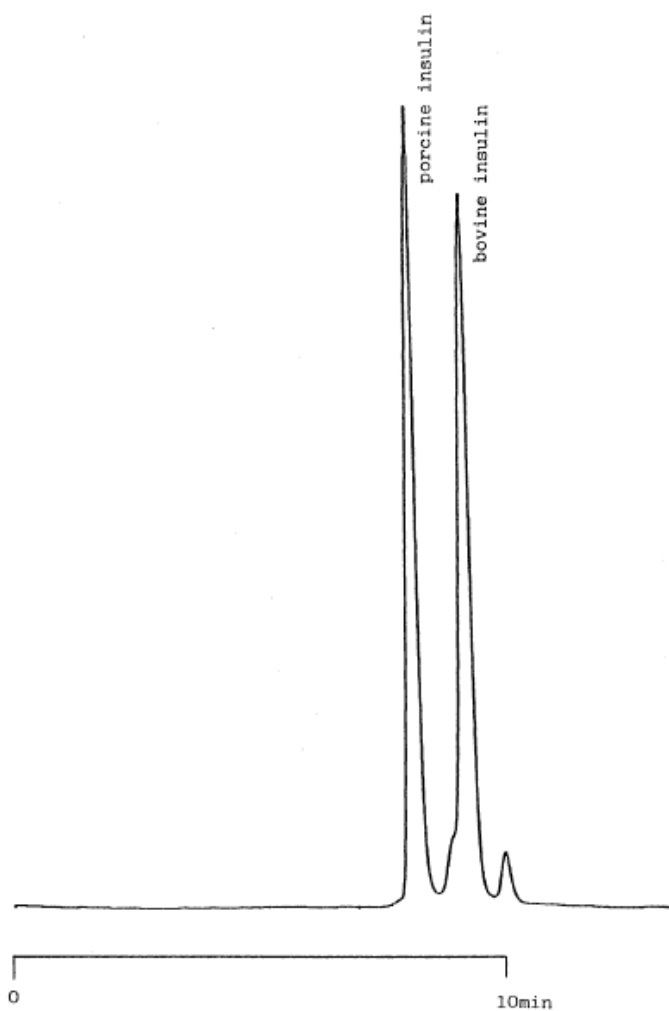

Column : Inertsil ODS-2  
5 $\mu$ m  
250  $\times$  4.6 mmI.D.  
Column Cat. No. : 5020-01102  
Eluent : A:0.1% CF<sub>3</sub>COOH in CH<sub>3</sub>CN  
B:0.1% CF<sub>3</sub>COOH  
A/B 20/80?(5min)?30/70  
→(40min)→50/50  
Flow rate : 1.0 mL/min.  
Col. Temp. : RT  
Detection : UV 280 nm  
Injection Vol. :  
Sample :  
Solutes :porcine insulin  
Bovine insulin