


InertSearch™ for LC

Inertsil® Applications


Analysis of Clomifene (2)

Data No. LA667-0142

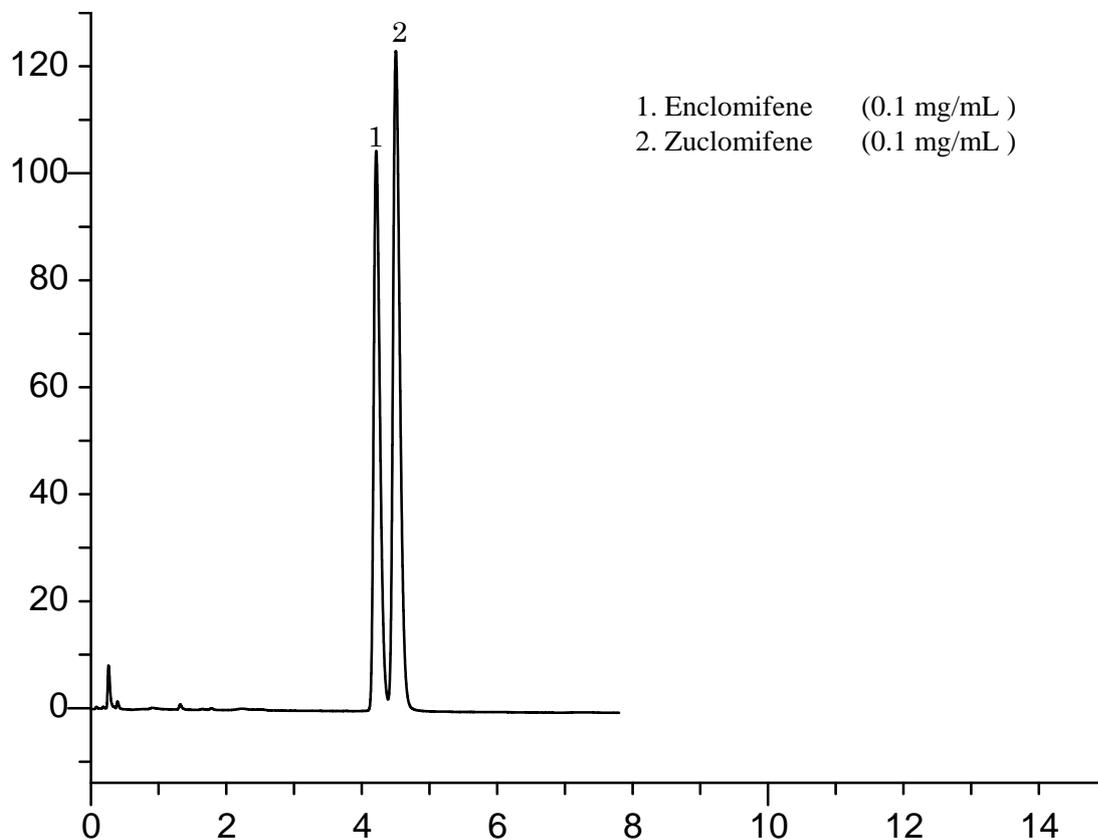


Conditions

System : LC800 HPLC system
Column : Inertsil ODS-3 (2 μ m, 75 x 2.1 mm I.D.)
Column Cat. No. : 5020-84653
Eluent : A) CH₃CN
B) 1 % Diethyl amine in H₂O (pH 6.2, H₃PO₄)
A/B = 50/50, v/v
Flow Rate : 0.6 mL/min
Col. Temp. : 40 °C
Detection : UV 233 nm (LC800 UV Detector)
Injection Vol. : 5 μ L
Sample : Clomifene citrate

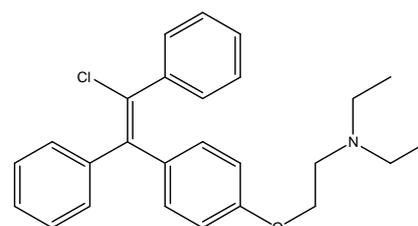

1. Enclomifene

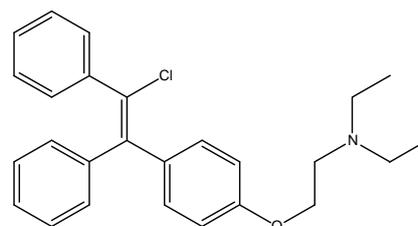

2. Zuclomifene