


Fermented foods like Miso, Sake, Syoyu made from cereals contain amino acids, organic acids, sugar and so on. In this study, they were extracted, derivatized, and analysed with gas chromatography/mass spectrometry. The silylated compounds in Miso, Sake and Syoyu extracts were identified using InertCap 5MS/NP metabolites Library (No.81).

### Procedure of sample preparation


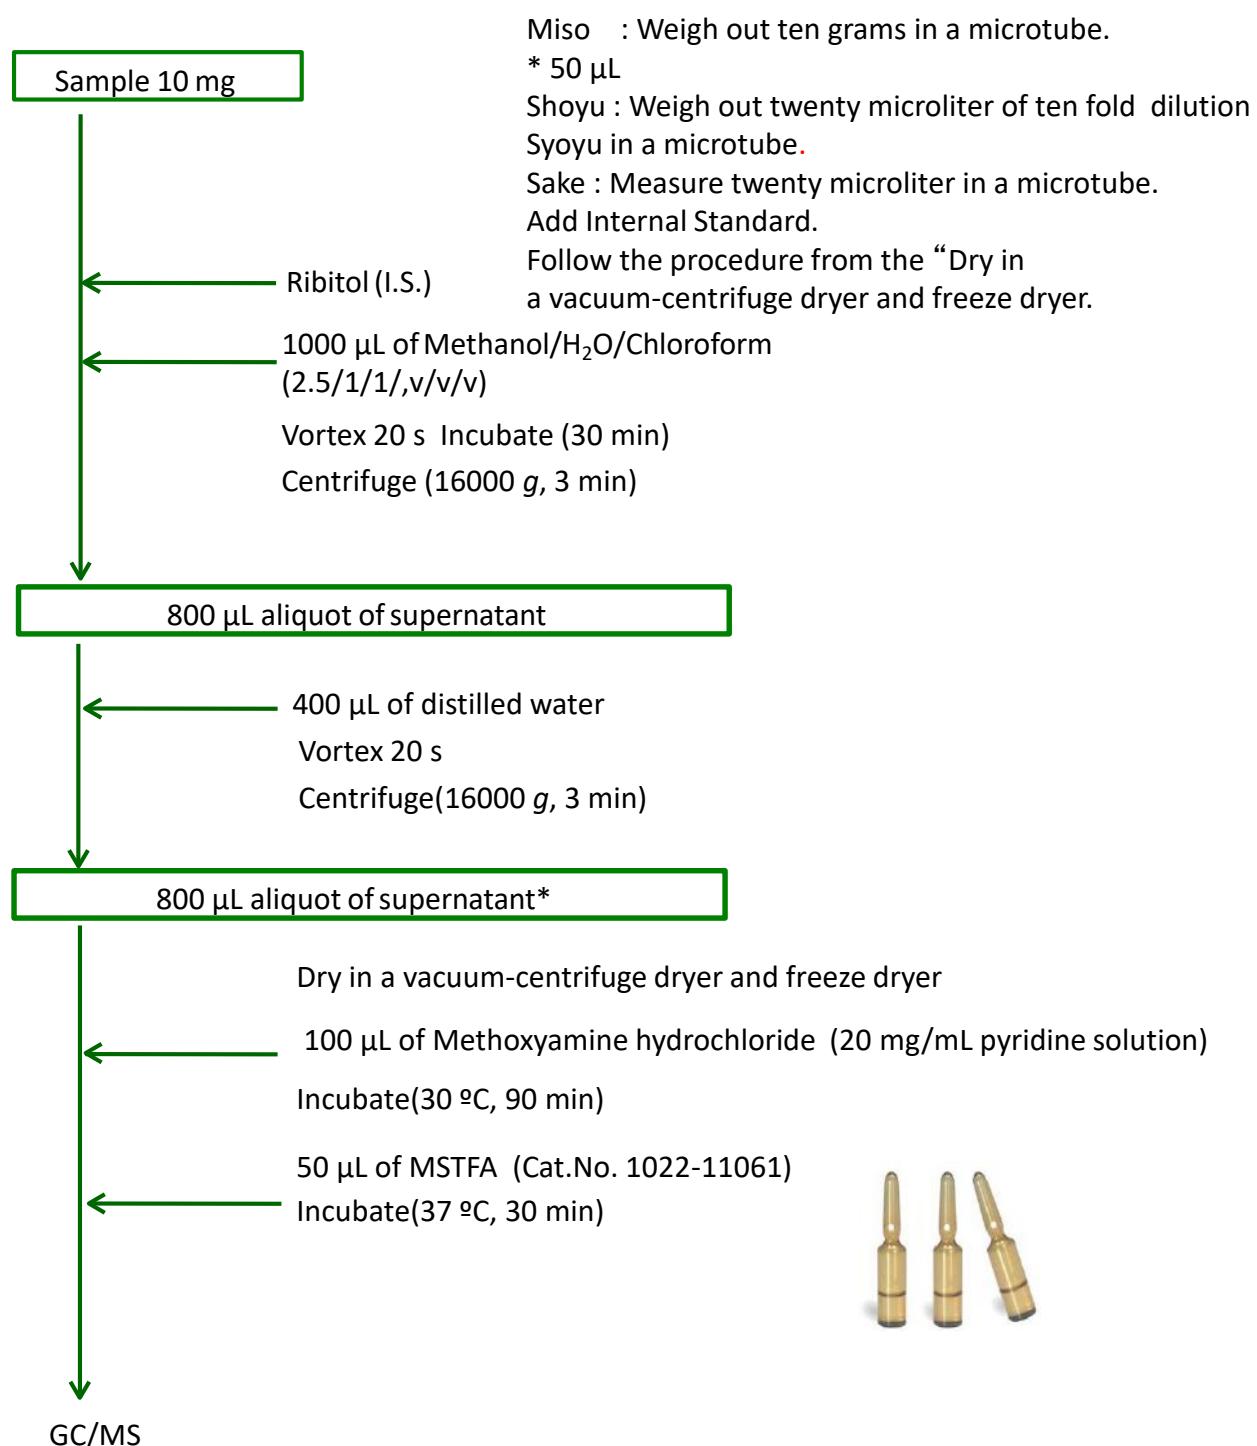


## Analysis of Miso

GC/MS Conditions

|                           |  |
|---------------------------|--|
| <b>System</b>             | : GC-MS  |
| <b>Column</b>             | : InertCap 5MS/NP 0.25 mm I.D. × 30 m df = 0.25 µm<br>(Cat.No. 1010-18642) |
| <b>Injection</b>          | : Split Constant Pressure 75 kPa   |
| <b>Injection Temp.</b>    | : 230 °C   |
| <b>Oven Temp.</b>         | : 80 °C (2 min) - 15 °C /min - 330 °C (13 min)                             |
| <b>Carrier gas</b>        | : Helium   |
| <b>Septum purge flow</b>  | : 5 mL/min   |
| <b>Split ratio</b>        | : 25:1   |
| <b>Interface Temp.</b>    | : 250 °C   |
| <b>Ion source Temp.</b>   | : 200 °C   |
| <b>Ionization Vortage</b> | : 70 eV  |
| <b>Scan range</b>         | : <i>m/z</i> 85 - 500  |
| <b>Inj. Vol.</b>          | : 1 µL   |

The silylated compounds in Miso extract were identified based on retention index and mass spectrum using InertCap metabolites library (Technical note No.81) and NIST.

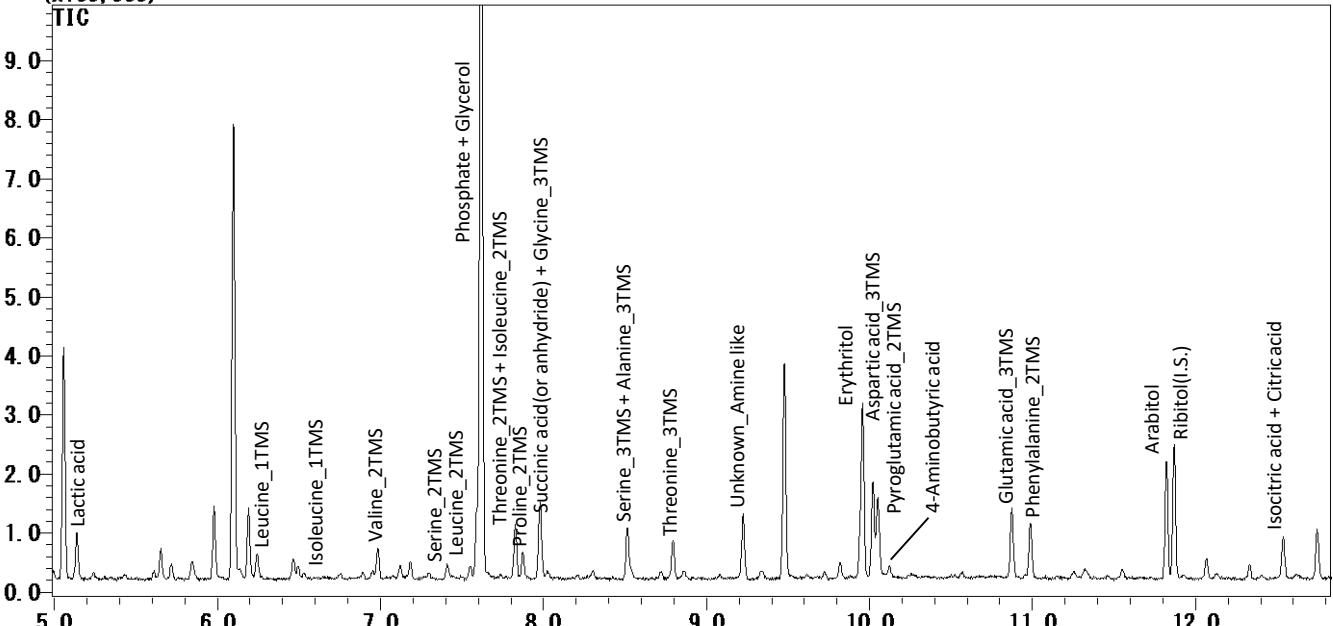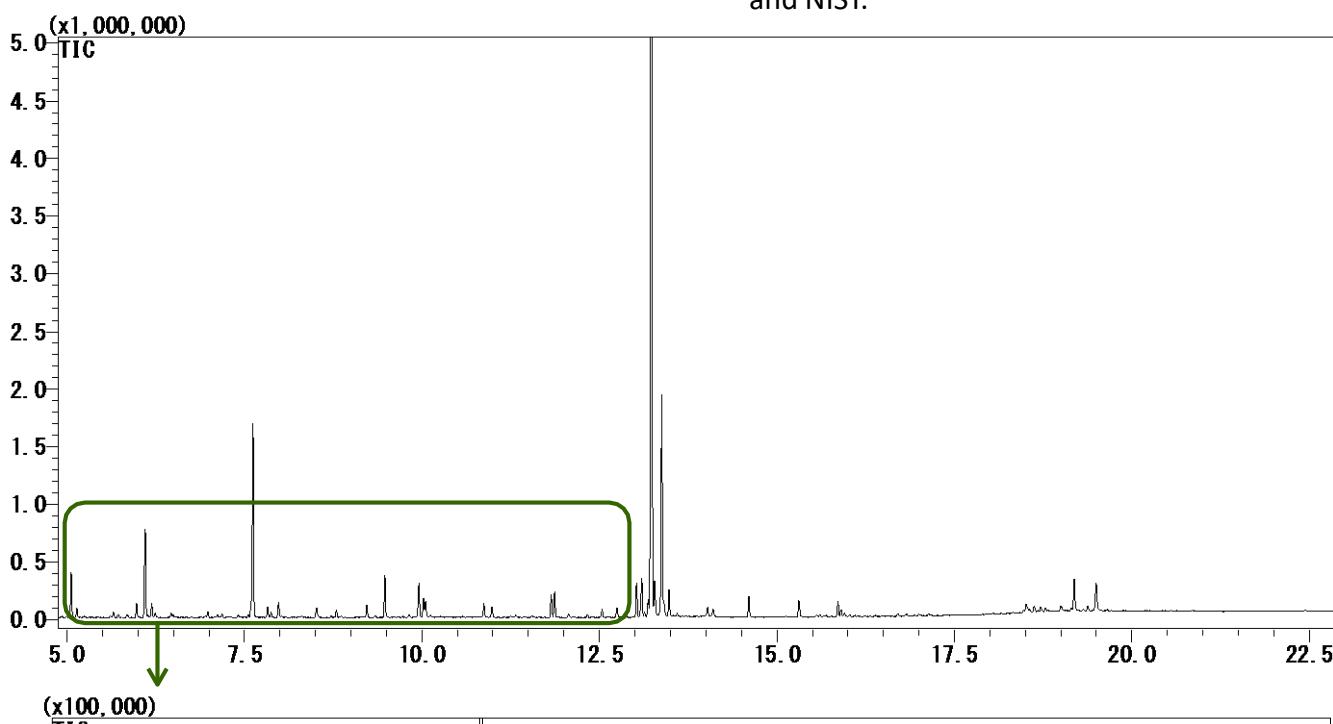

## Analysis of Sake

GC/MS Conditions

## System Column

: GC-MS

: InertCap 5MS/NP 0.25 mm I.D. × 30 m df = 0.25 µm  
(Cat.No. 1010-18642)

## Injection

: Split Constant Pressure 75 kPa

## Inj. Temp.

: 230 °C

## Oven Temp.

: 80 °C (2 min) - 15 °C /min - 330 °C (13 min)

## Carrier gas

: Helium

## Septum purge flow

: 5 mL/min

## Split ratio

: 25:1

## Interface Temp.

: 250 °C

## Ion source Temp.

: 200 °C

## Ionization Vortage

: 70 eV



## Scan range

: *m/z* 85 - 500

## Inj. Vol.

: 1 µL

The silylated compounds in Sake extract were identified based on retention index and mass spectrum using InertCap metabolites library (Technical note No.81) and NIST.

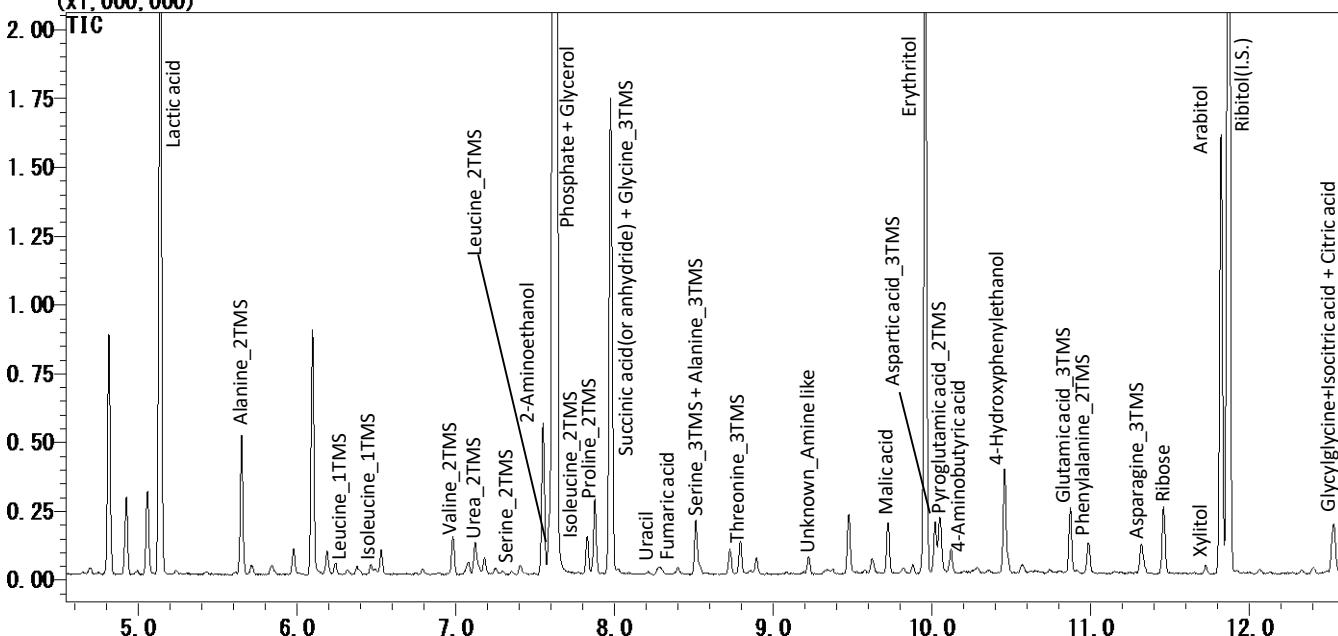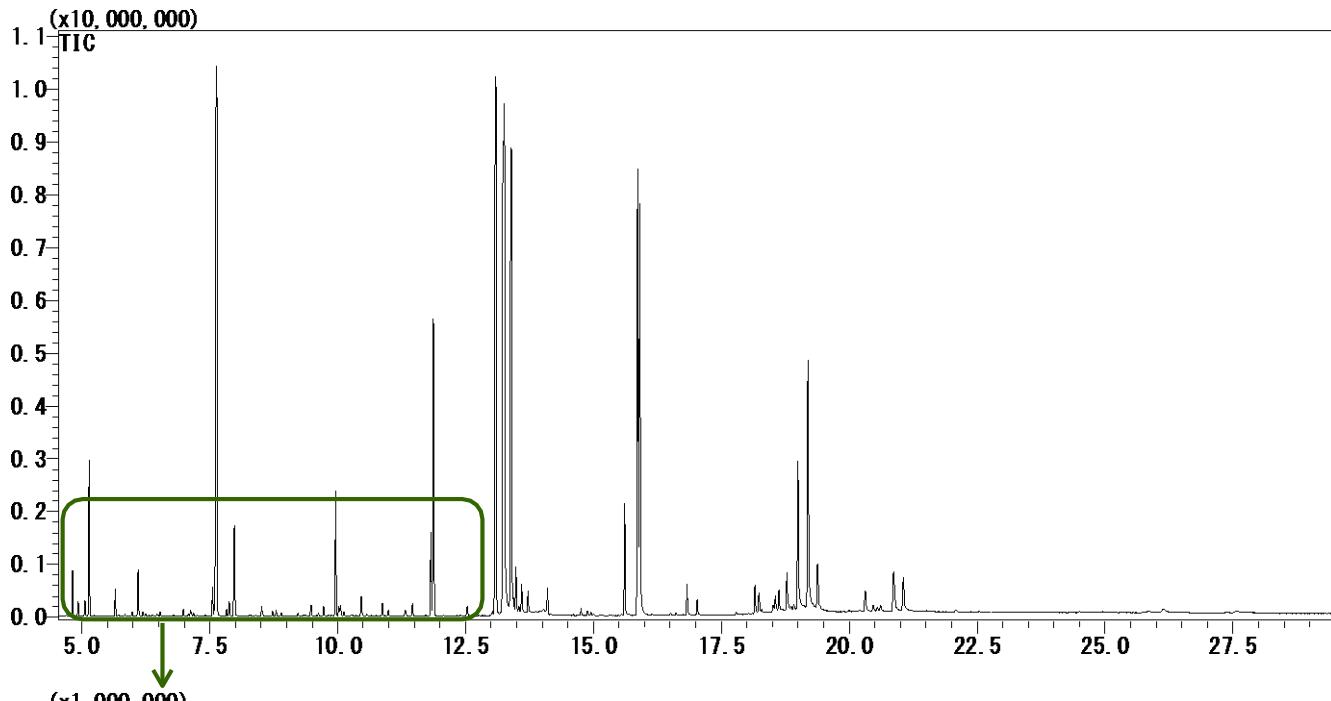



## Analysis of Syoyu

## GC/MS Conditions

## System Column

: GC-MS  
 : InertCap 5MS/NP 0.25 mm I.D. × 30 m df = 0.25 µm  
 (Cat.No. 1010-18642)  
 : Split Constant Pressure 75 kPa  
 : 230 °C  
 : 80 °C (2 min) - 15 °C /min - 330 °C (13 min)  
 : Helium  
 : 5 mL/min  
 : 25:1  
 : 250 °C  
 : 200 °C  
 : 70 eV  
 : *m/z* 85 - 500  
 : 1 µL

The silylated compounds in Syoyu extract were identified based on retention index and mass spectrum using InertCap metabolites library (Technical note No.81) and NIST.

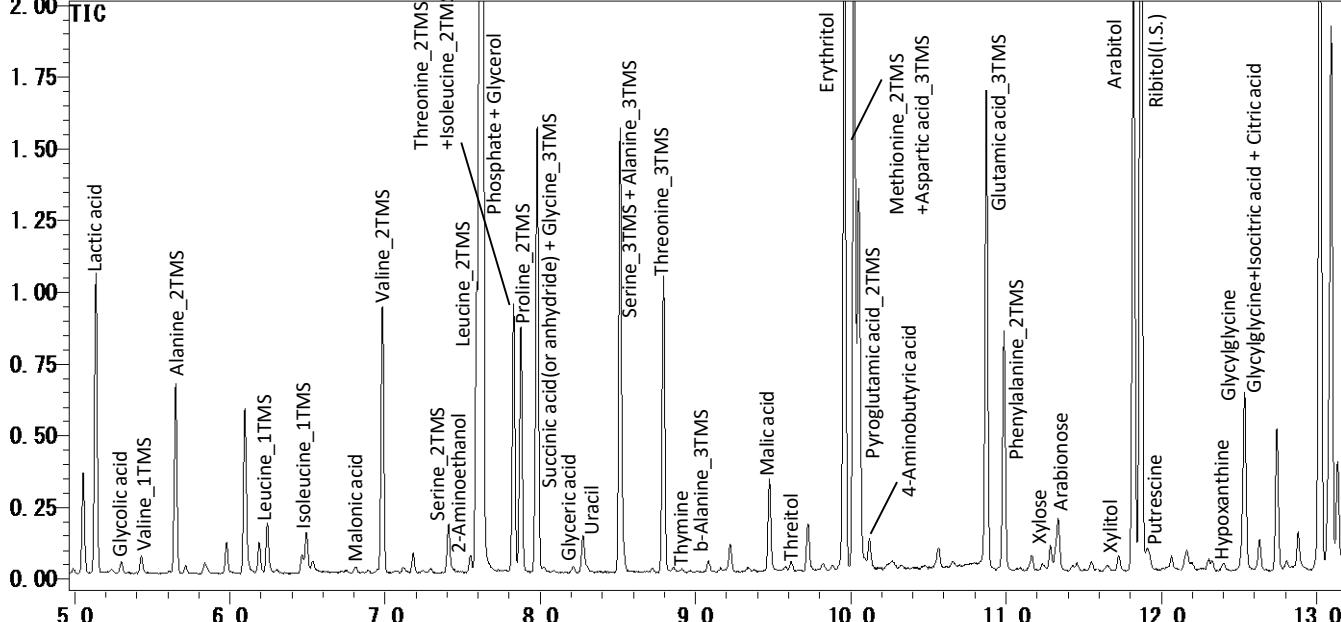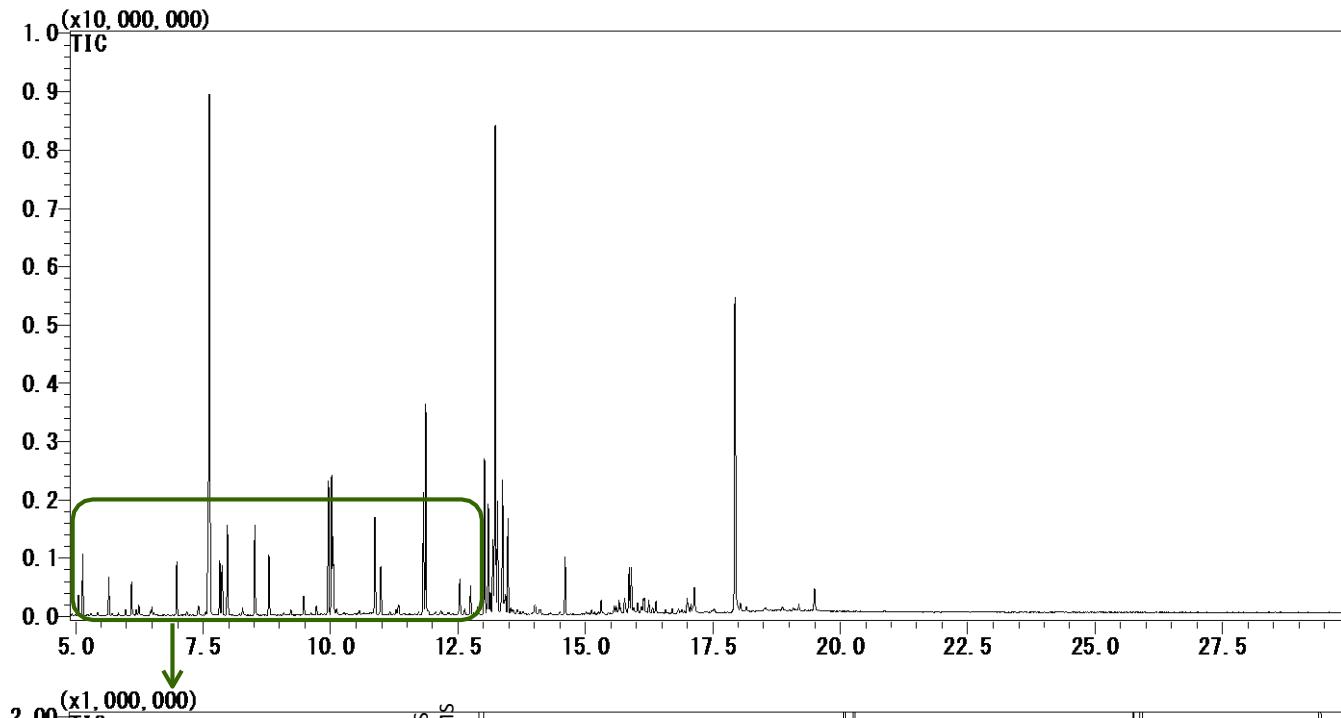

Aloutput is available for peak identification. In that case, it is convenient to use the *n*-alkane standard solution C9-C40 in *n*- Hexane.

### What is Aloutput?

- Software for metabolome analyses based on Excel (upto 2007)
- Peak identification based on retention indices and mass spectrum
- Auto peak identification, PCA analysis, PLS analysis, t-test
- Free software!
- Everybody can download, now!

[http://prime.psc.riken.jp/Metabolomics\\_Software/Aloutput/index.html](http://prime.psc.riken.jp/Metabolomics_Software/Aloutput/index.html)


### *n*-Alkane standard solution C9-C40 in *n*-Hexane

Concentration: 50 µg/mL each component of *n*-Hexane

※C10,C20,C30,C40 are 100 µg/mL

Volume: 1 mL

Packaging: ampule of 1 mL

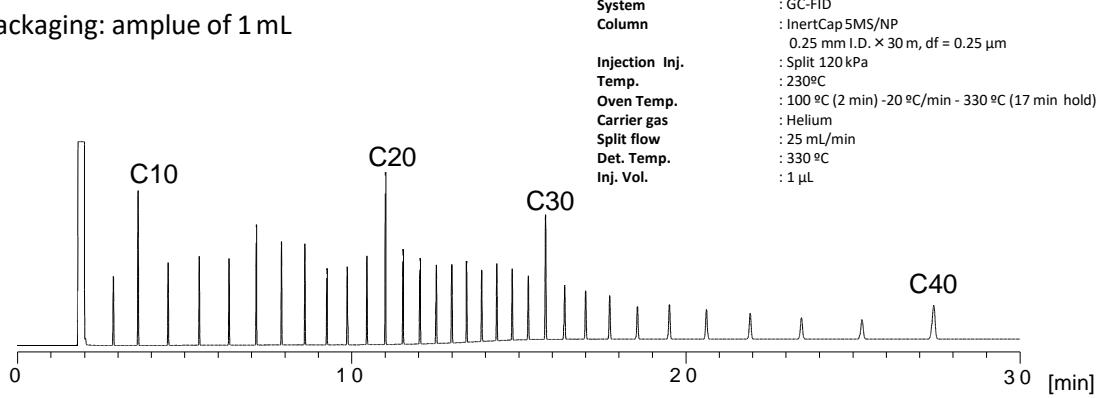

| Description   | Volume   | Cat.No.    |
|---|----------|------------|
| <i>n</i> -Alkane standard solution C9-C40 in C6 (cold strage) | 1 mL     | 1021-58321 |
|   | 1 mL × 5 | 1021-58325 |

This product contains hazardous material which requires special freight handling, and then additional charges apply. Please contact your local distributor.

GL Sciences disclaims any and all responsibility for any injury or damage which may be caused by this data directly or indirectly. We reserve the right to amend this information or data at any time and without any prior announcement.

GL Sciences disclaims any and all responsibility for any injury or damage which may be caused by this data directly or indirectly. We reserve the right to amend this information or data at any time and without any prior announcement.

### GL Sciences, Inc. Japan

22-1 Nishishinjuku 6-Chome  
Shinjuku-ku, Tokyo,  
163-1130, Japan  
Phone: +81-3-5323-6620  
Fax: +81-3-5323-6621  
Email: [world@glsci.co.jp](mailto:world@glsci.co.jp)  
Web: [www.glsciences.com](http://www.glsciences.com)

### GL Sciences B.V.

De Sleutel 9  
5652 AS Eindhoven  
The Netherlands  
Phone: +31 (0)40 254 95 31  
Email: [info@glsciences.eu](mailto:info@glsciences.eu)  
Web: [www.glsciences.eu](http://www.glsciences.eu)

### GL Sciences (ShangHai) Ltd.

Tower B, Room 2003,  
Far East International Plaza,  
NO,317 Xianxia Road,  
Changning District.  
Shanghai, China P.C. 200032  
Phone: +86 (0)21-6278-2272  
Email: [contact@glsciences.com.cn](mailto:contact@glsciences.com.cn)  
Web: [www.glsciences.com.cn](http://www.glsciences.com.cn)

### GL Sciences, Inc. USA

4733 Torrance Blvd. Suite 255  
Torrance, CA 90503  
Phone: 310-265-4424  
Fax: 310-265-4425  
Email: [info@glsciencesinc.com](mailto:info@glsciencesinc.com)  
Web: [www.glsciencesinc.com](http://www.glsciencesinc.com)

### International Distributors

Visit our Website at:  
[https://www.glsciences.com/company/distributor.html](http://www.glsciences.com/company/distributor.html)

