


Analysis of Febuxostat


(Under the Condition of the Japanese Pharmacopoeia 18th Supplement II, Febuxostat, Related substances (i))

Test for required detectability

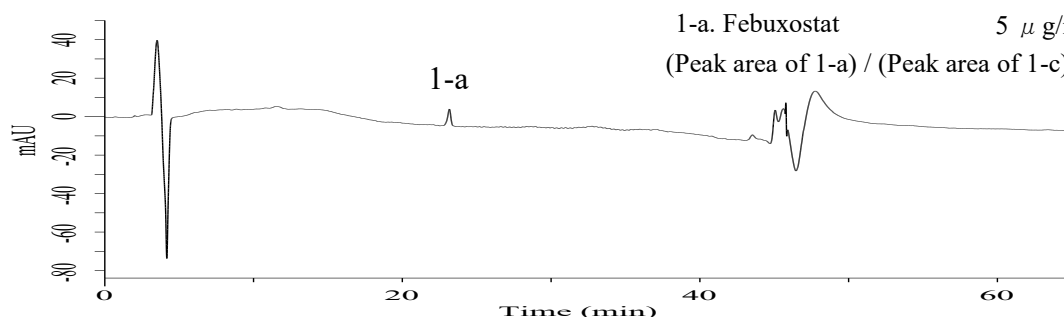


1-a. Febuxostat 5 μ g/mL
 (Peak area of 1-a) / (Peak area of 1-c) : $(7 \leq) 8.68 (\leq 13)$

System performance

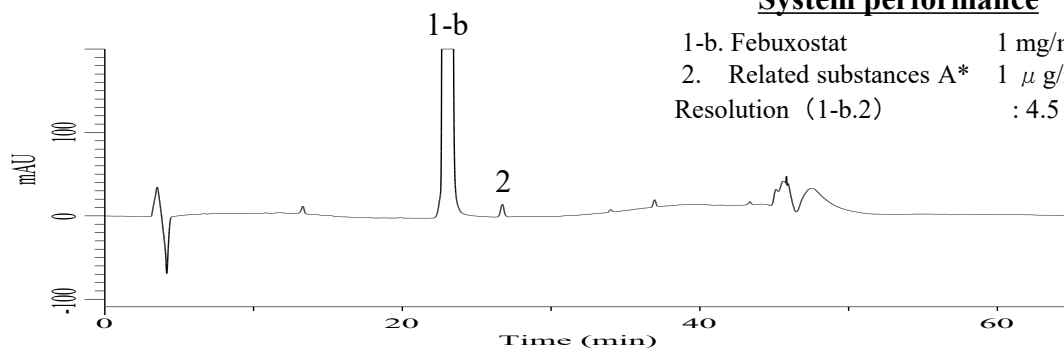

1-b. Febuxostat 1 mg/mL
 2. Related substances A* 1 μ g/mL
 Resolution (1-b.2) : $4.5 (\geq 2.0)$

System repeatability

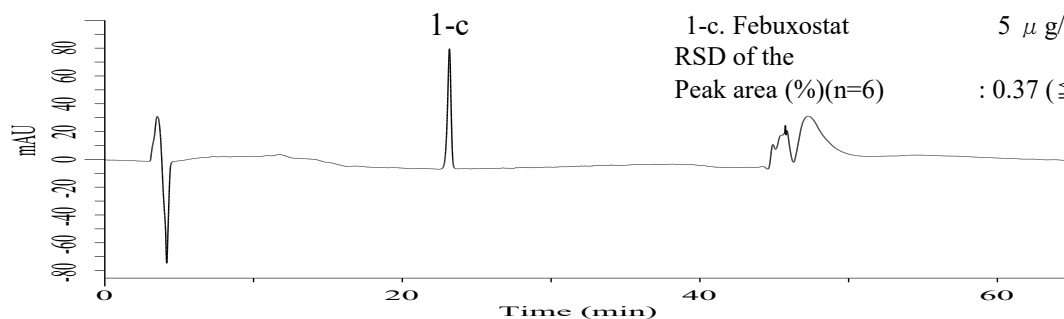

1-c. Febuxostat 5 μ g/mL
 RSD of the
 Peak area (%)(n=6) : $0.37 (\leq 2.0)$

Conditions

System : Chromaster HPLC system (HITACHI)
Column : InertSustain AQ-C18 (GL Sciences Inc.)
 (5 μ m, 250 x 4.6 mm I.D.)
Column Cat. No. : 5020-89731
Eluent : A) 0.02% CH₃COOH in H₂O
 B) 0.02% CH₃COOH in CH₃CN

Time(min)	A(vol%)	B(vol%)
0.0	60	40
40.0	0	100

Flow Rate : 0.70 mL/min
Col. Temp. : 40 °C
Detection : UV 217 nm
Injection Vol. : 40 μ L
Sample : Standard

Analyte:

1. Febuxostat
 2. Related substances A*

* 2-[3-Ethoxycarbonyl-4-(2-methylpropoxy)phenyl]-4-methyl-1,3-thiazole-5-carboxylic acid