


# InertSearch™ for LC

Inertsil® Applications

## Analysis of Vitamin D

Data No. LB808-7111

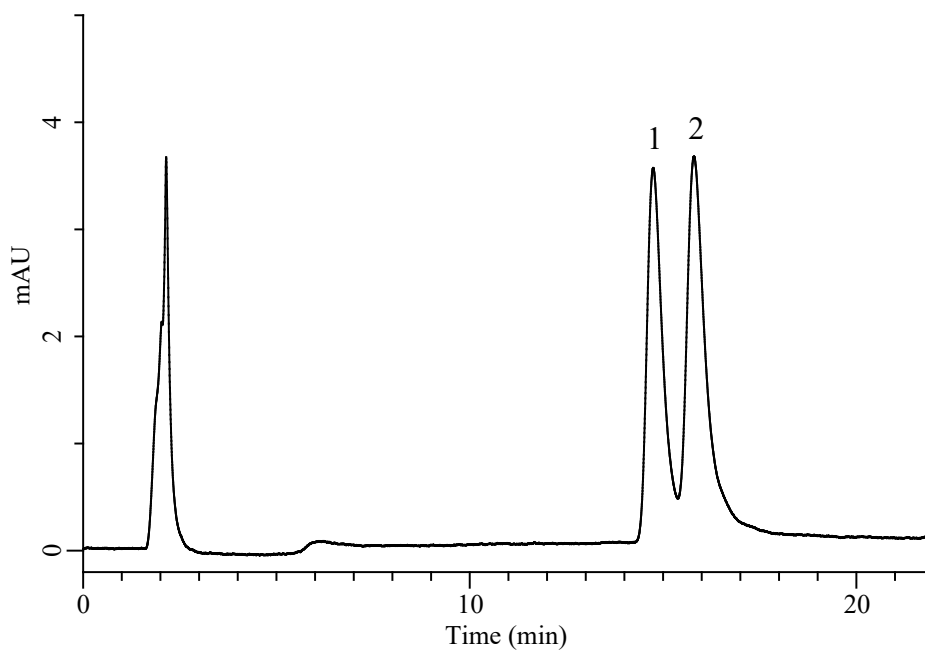

### Conditions

**System** : Chromaster HPLC system (HITACHI)

**Column** : InertSustain C30 (GL Sciences Inc.)  
(HP 3  $\mu$  m, 250 x 3.0 mm I.D.)

**Column Cat. No.** : 5020-17181

**Eluent** : CH<sub>3</sub>CN

**Flow Rate** : 0.6 mL/min

**Col. Temp.** : 25 °C

**Detection** : UV 265 nm

**Injection Vol.** : 5  $\mu$  L

**Sample** : Standard

### Analyte:

1. Vitamin D2 5 mg/L

2. Vitamin D3 5 mg/L