


InertSearch™ for GC

InertCap® Applications

Moldy odors

Data No. GA025-0000

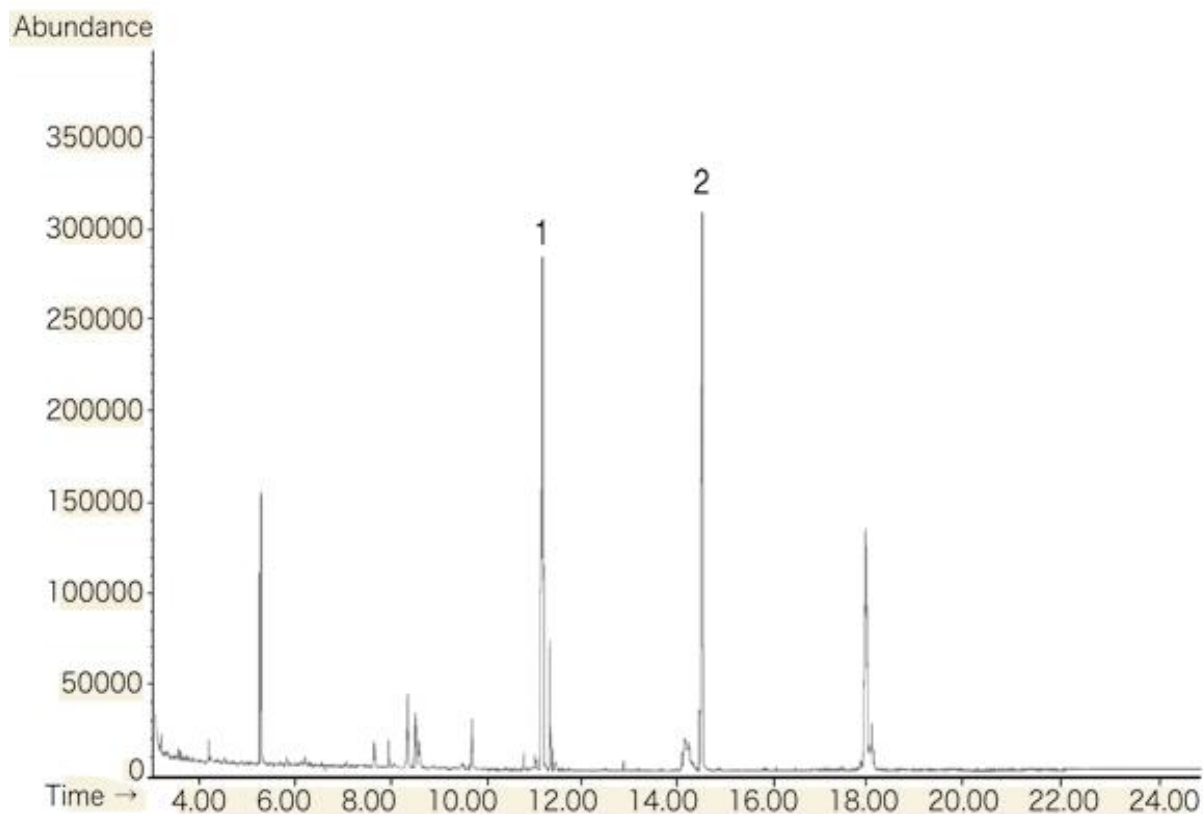

System :GC/MS P&T

Column :InertCap 1
0.25mmI.D.×30m df=0.4µm

Column Temp. :40°C (1min Hold)→10°C/min→220°C

Carrier Gas :He 70kPa

Injection :P&T

Detection :MS

Sample :1µg/L

Solutes : 1. 2-MIB (2-Methyl-isoborneol)

2. Geosmine