


31. Analysis of Aflatoxin

Data No. LA086-0000

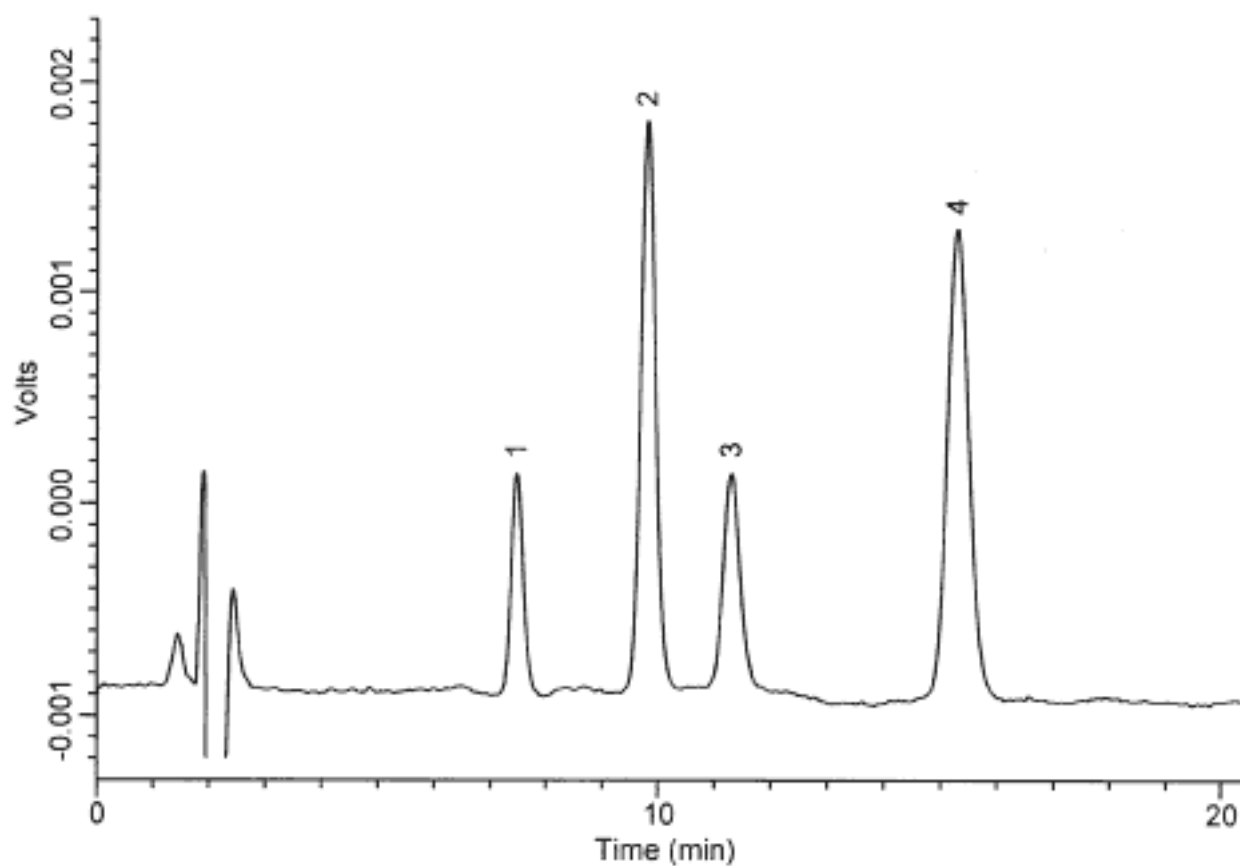

| | | | |
|-------------------|--|---------|--|
| Column | :Inertsil C8-3 150 × 4.6 mm I.D. | Solutes | : 1. Aflatoxin G2 (0.06 µg/mL) 2. Aflatoxin G1 (0.20 µg/mL) |
| Column Cat. No. : | | | 3. Aflatoxin B2 (0.06 µg/mL) |
| Eluent | :CH ₃ OH/H ₂ O = 40/60 | | 4. Aflatoxin B1 (0.20 µg/mL) |
| Flow rate | :1.0 mL/min. | | |
| Col. Temp. | :40°C | | |
| Detection | :UV 365 nm | | |
| Injection Vol. | :100 µL | | |
| Sample | :Aflatoxins | | |