


## Analysis of PA(Pyridylaminated) oligosaccharides

Data No. LA828-0699

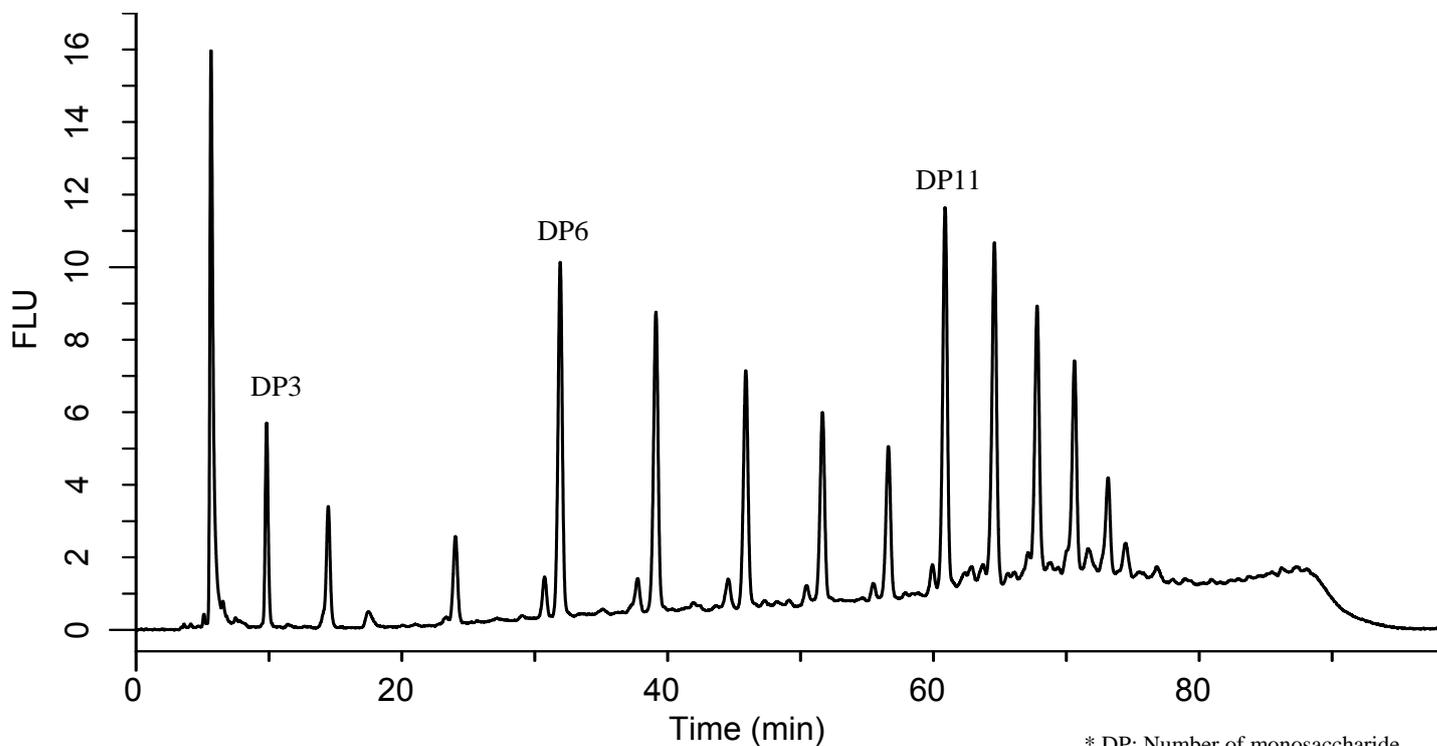

### Conditions

**System** : GL-7400 HPLC System  
**Column** : MonoClad C18-HS (150 x 3.0 mm I.D.)  
**Column Cat. No.** : 5020-10803  
**Eluent** : A) CH<sub>3</sub>CN/ H<sub>2</sub>O/TFA = 20/80/0.02  
          : B) H<sub>2</sub>O/TFA = 100/0.02  
          : A/B = 0/100 - 5 min - 0/100 - 65 min - 10/90 - 10 min - 15/85, v/v  
**Flow Rate** : 0.3 mL/min  
**Col. Temp.** : FL Ex 310 nm Em 380 nm (GL-7453A FL Detector)  
**Detection** : 30 °C  
**Injection Vol.** : 5 µL  
**Sample** : PA-Glucose oligomer (DP = 3 - 15)