


InertSearch™ for LC

Inertsil® Applications

Analysis of Oxalic acid

Data No. LB003-0721

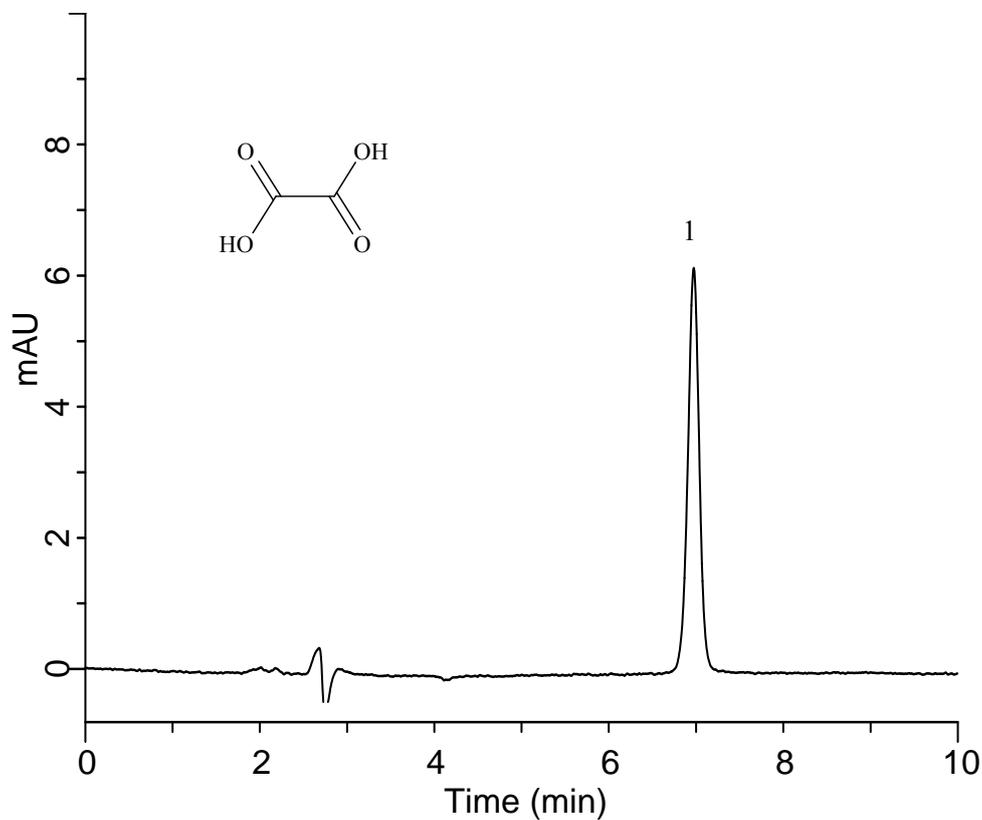

Conditions

System : GL-7400 HPLC system
Column : Inertsil Amide (5 μm, 250 x 4.6 mm I.D.)
Column Cat. No. : 5020-07836
Eluent : A) CH₃CN
 : B) 30 mM Na₂HPO₄(pH 6.8)
 : A/B = 65/35, v/v
Flow rate : 1 mL/min
Col. Temp. : 50 °C
Detection : UV 220 nm (GL-7450 UV Detector)
Injection Vol. : 5 μL
Sample : Standard

Analyte:

1. Oxalic acid 100 mg/L